

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082524\
 Data File : PD084656.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2024 01:14
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 05:29:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 23 05:28:46 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.906	9971844	35727876	9.841	10.086
27)	SA Decachlor...	9.032	8.107	26434489	72628337	20.154	20.694
Target Compounds							
2)	A alpha-BHC	3.983	3.417	15447827	50150942	9.279	9.824
3)	MA gamma-BHC...	4.311	3.752	14877706	48512587	9.352	9.973
4)	MA Heptachlor	4.909	4.107	14352876	42438452	9.500	9.888
9)	A Endosulfan I	6.051	5.273	13233817	38941923	9.639	10.040
13)	MA Dieldrin	6.323	5.540	27393626	86496096	18.727	19.947
14)	MA Endrin	6.551	5.818	20461644	74175707	18.708	19.896
16)	A 4,4'-DDD	6.680	5.958	18322372	68154457	18.729	19.905
17)	MA 4,4'-DDT	6.996	6.213	16181948	62594898	18.268	19.364
20)	A Methoxychlor	7.466	6.785	49520585	172.5E6	94.334	102.317


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082524\
Data File : PD084656.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2024 01:14
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 05:29:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Fri Aug 23 05:28:46 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

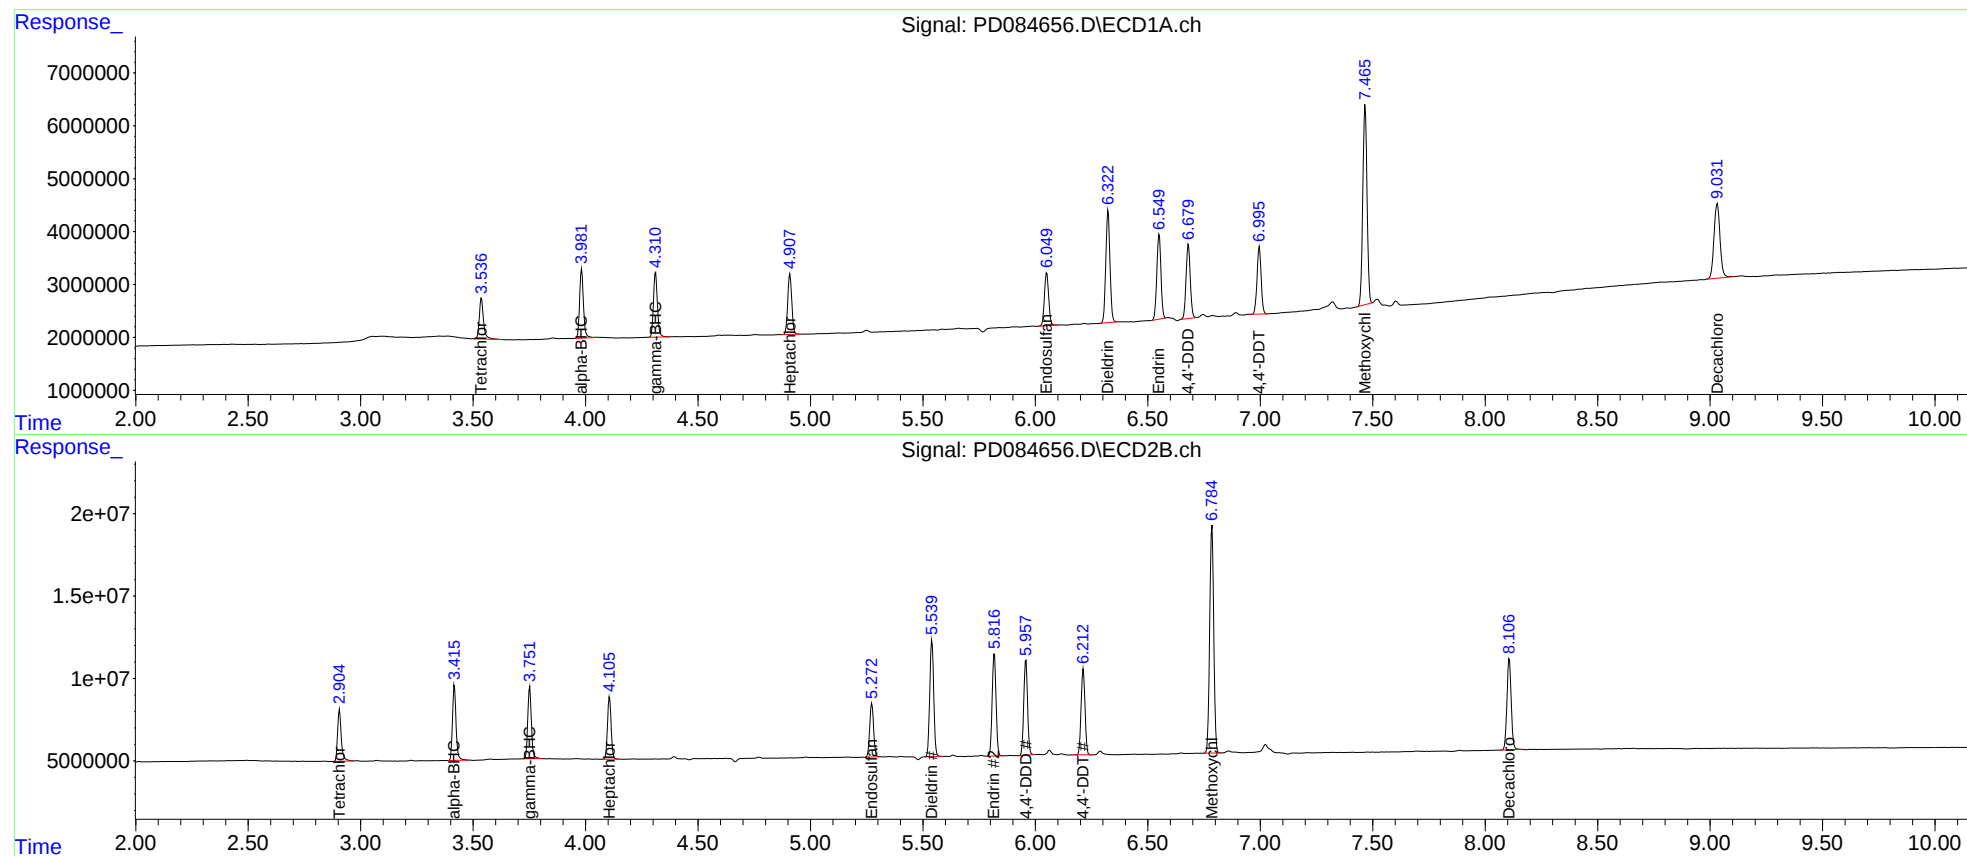

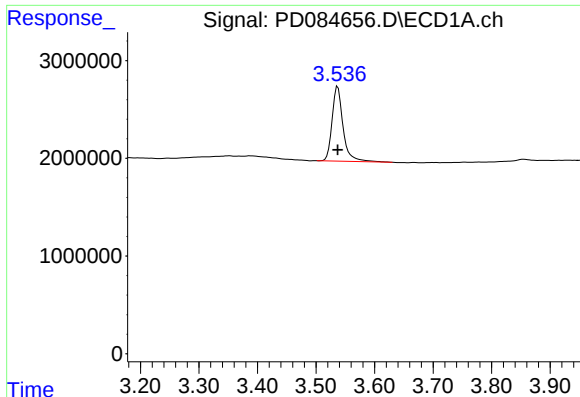


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 9971844
Conc: 9.84 ng/ml

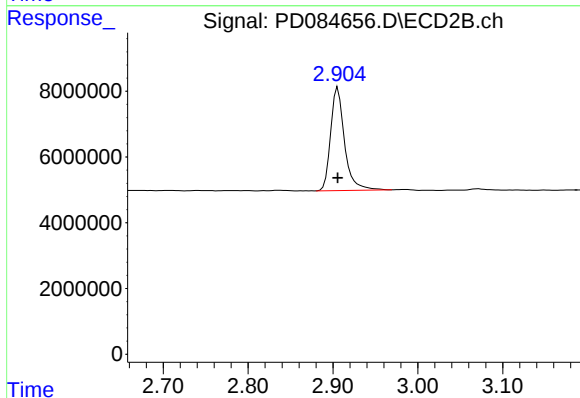


#1 Tetrachloro-m-xylene

R.T.: 2.906 min
Delta R.T.: 0.000 min
Response: 35727876
Conc: 10.09 ng/ml

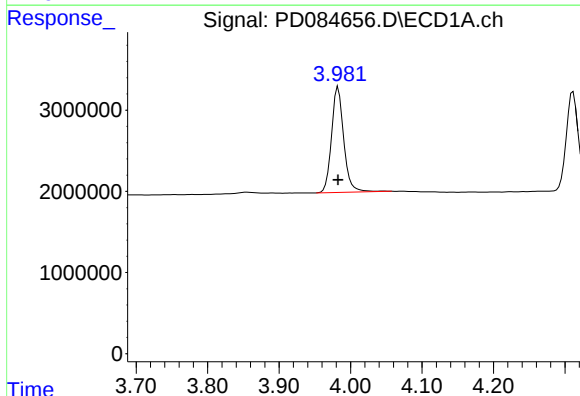


#2 alpha-BHC

R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 15447827
Conc: 9.28 ng/ml

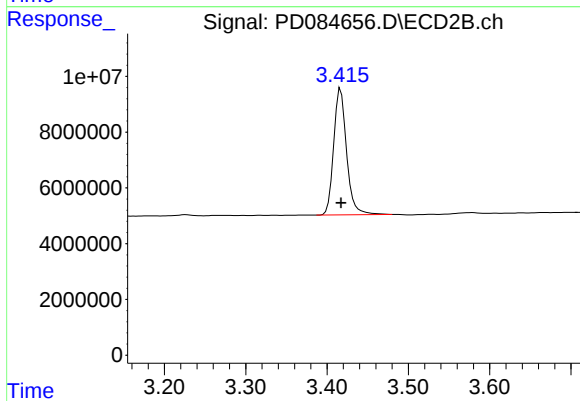


#2 alpha-BHC

R.T.: 3.417 min
Delta R.T.: 0.000 min
Response: 50150942
Conc: 9.82 ng/ml

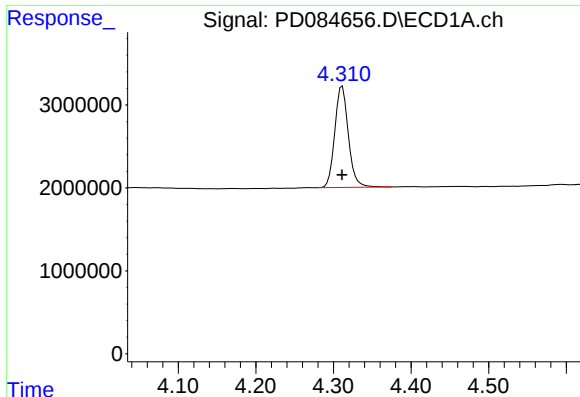


#3 gamma-BHC (Lindane)

R.T.: 4.311 min
Delta R.T.: 0.000 min
Response: 14877706
Conc: 9.35 ng/ml

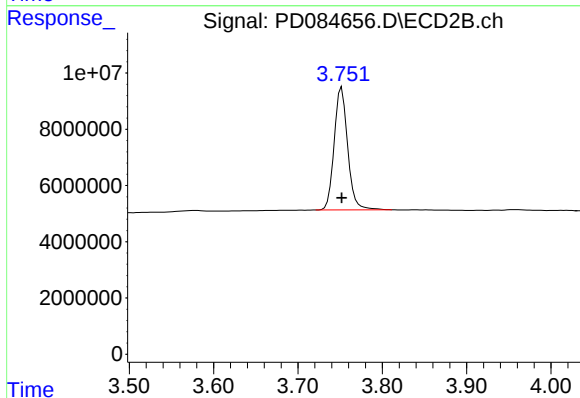


#3 gamma-BHC (Lindane)

R.T.: 3.752 min
Delta R.T.: 0.000 min
Response: 48512587
Conc: 9.97 ng/ml

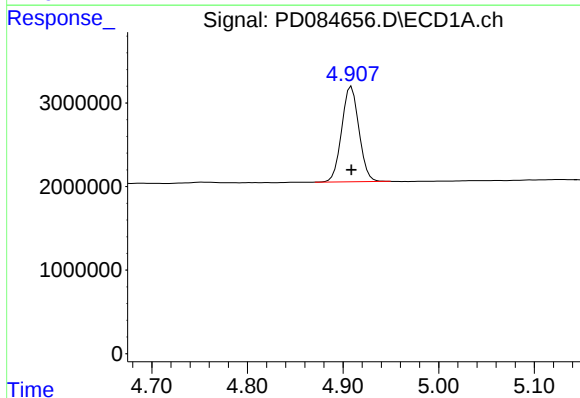


#4 Heptachlor

R.T.: 4.909 min
Delta R.T.: 0.000 min
Response: 14352876
Conc: 9.50 ng/ml

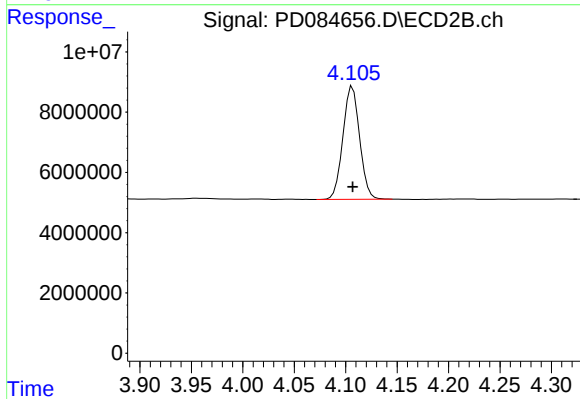


#4 Heptachlor

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 42438452
Conc: 9.89 ng/ml

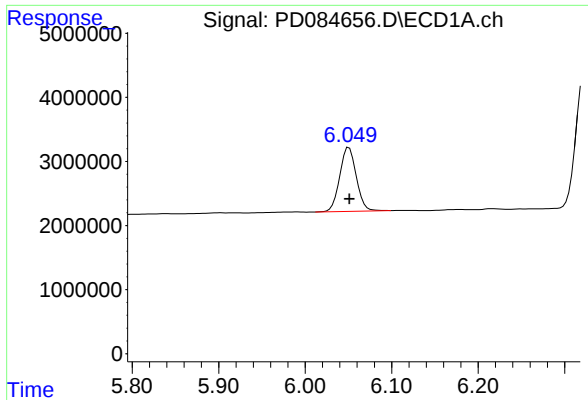


#9 Endosulfan I

R.T.: 6.051 min
Delta R.T.: 0.000 min
Response: 13233817
Conc: 9.64 ng/ml

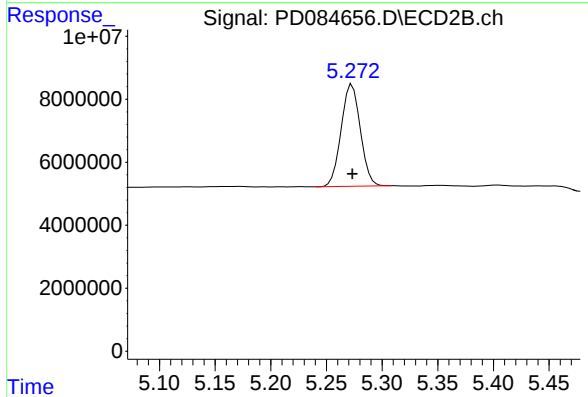


#9 Endosulfan I

R.T.: 5.273 min
Delta R.T.: 0.000 min
Response: 38941923
Conc: 10.04 ng/ml

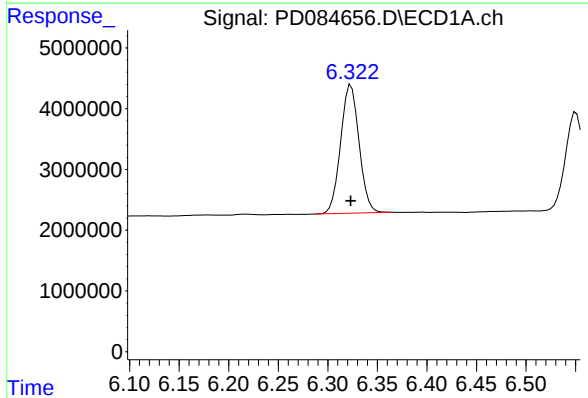


#13 Dieldrin

R.T.: 6.323 min
Delta R.T.: 0.000 min
Response: 27393626
Conc: 18.73 ng/ml

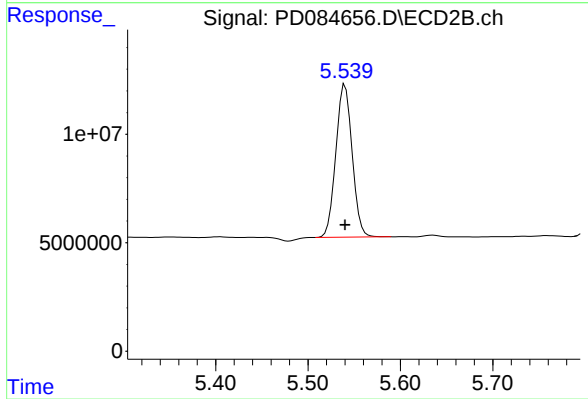


#13 Dieldrin

R.T.: 5.540 min
Delta R.T.: 0.000 min
Response: 86496096
Conc: 19.95 ng/ml

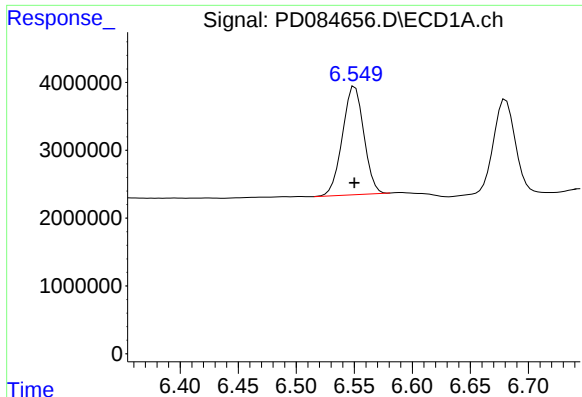


#14 Endrin

R.T.: 6.551 min
Delta R.T.: 0.000 min
Response: 20461644
Conc: 18.71 ng/ml

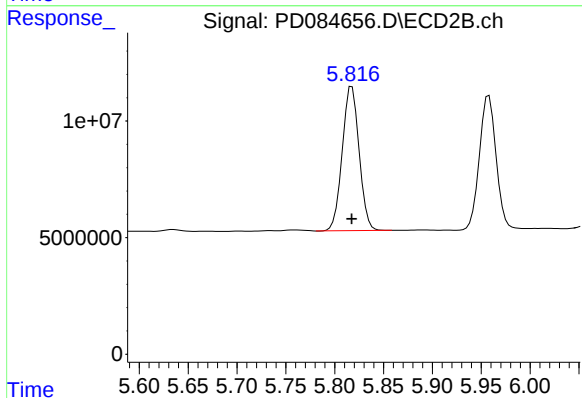


#14 Endrin

R.T.: 5.818 min
Delta R.T.: 0.000 min
Response: 74175707
Conc: 19.90 ng/ml

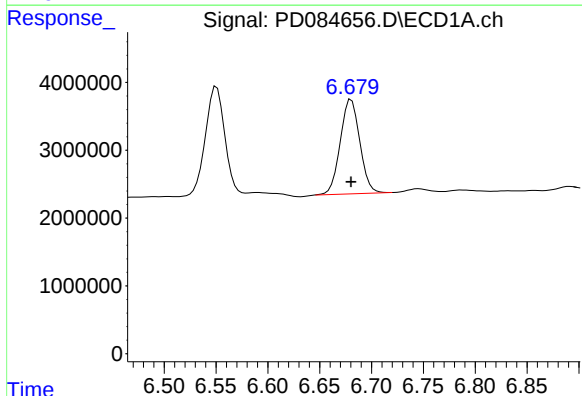


#16 4,4'-DDD

R.T.: 6.680 min
Delta R.T.: 0.000 min
Response: 18322372
Conc: 18.73 ng/ml

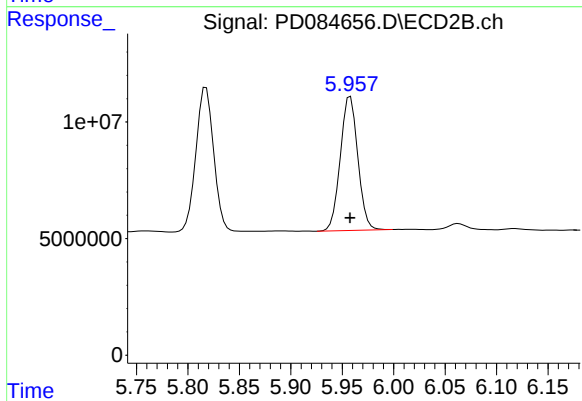


#16 4,4'-DDD

R.T.: 5.958 min
Delta R.T.: 0.000 min
Response: 68154457
Conc: 19.90 ng/ml

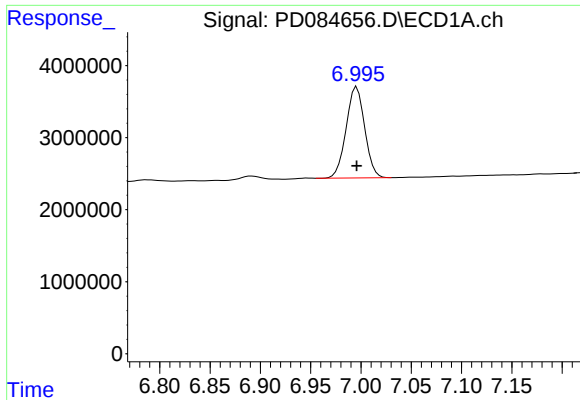


#17 4,4'-DDT

R.T.: 6.996 min
Delta R.T.: 0.000 min
Response: 16181948
Conc: 18.27 ng/ml

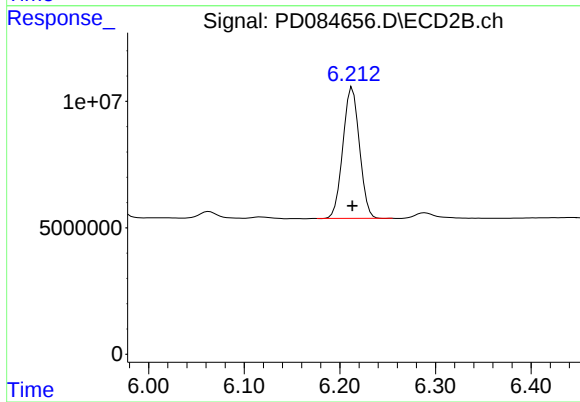


#17 4,4'-DDT

R.T.: 6.213 min
Delta R.T.: 0.000 min
Response: 62594898
Conc: 19.36 ng/ml

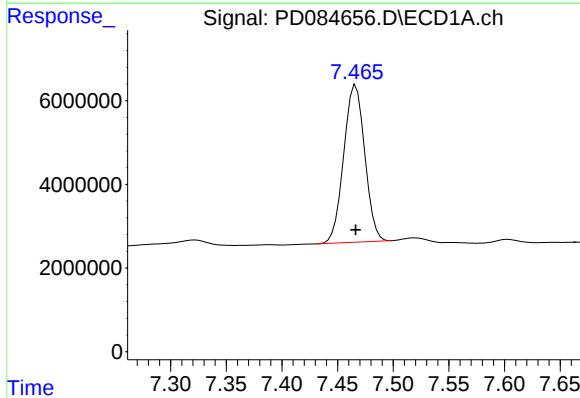


#20 Methoxychlor

R.T.: 7.466 min
Delta R.T.: 0.000 min
Response: 49520585
Conc: 94.33 ng/ml

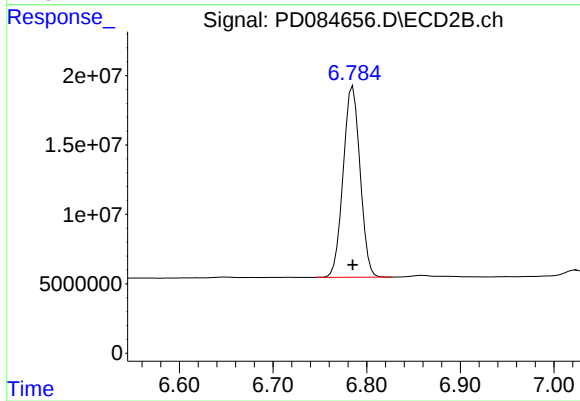


#20 Methoxychlor

R.T.: 6.785 min
Delta R.T.: 0.000 min
Response: 172542765
Conc: 102.32 ng/ml

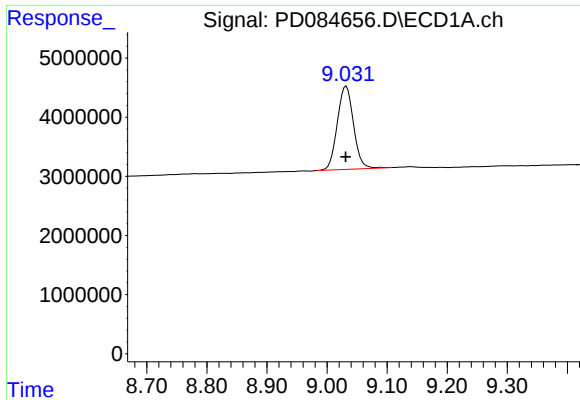

#27 Decachlorobiphenyl

R.T.: 9.032 min
Delta R.T.: 0.000 min
Response: 26434489
Conc: 20.15 ng/ml

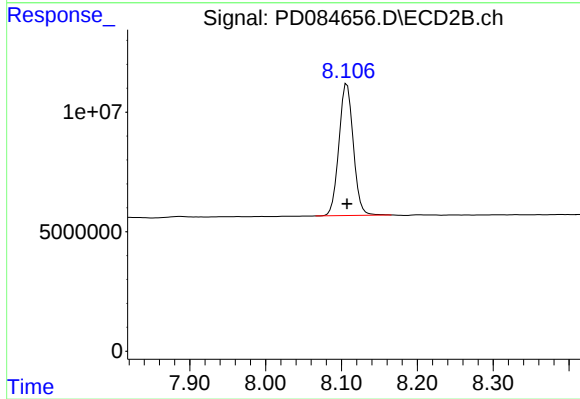

#27 Decachlorobiphenyl

R.T.: 8.107 min
Delta R.T.: 0.000 min
Response: 72628337
Conc: 20.69 ng/ml