

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082524\
 Data File : PD084658.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2024 01:41
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 05:29:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 23 05:28:46 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.906	20264891	70845388	20.000	20.000
27)	SA Decachlor...	9.031	8.107	52465345	140.4E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.983	3.417	33294943	102.1E6	20.000	20.000
3)	MA gamma-BHC...	4.311	3.752	31815775	97284049	20.000	20.000
4)	MA Heptachlor	4.909	4.107	30216696	85840361	20.000	20.000
9)	A Endosulfan I	6.051	5.273	27458666	77570570	20.000	20.000
13)	MA Dieldrin	6.323	5.540	58511743	173.4E6	40.000	40.000
14)	MA Endrin	6.550	5.817	43748411	149.1E6	40.000	40.000
16)	A 4,4'-DDD	6.680	5.958	39131439	137.0E6	40.000	40.000
17)	MA 4,4'-DDT	6.996	6.213	35433115	129.3E6	40.000	40.000
20)	A Methoxychlor	7.466	6.785	105.0E6	337.3E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082524\
Data File : PD084658.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2024 01:41
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 05:29:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Fri Aug 23 05:28:46 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

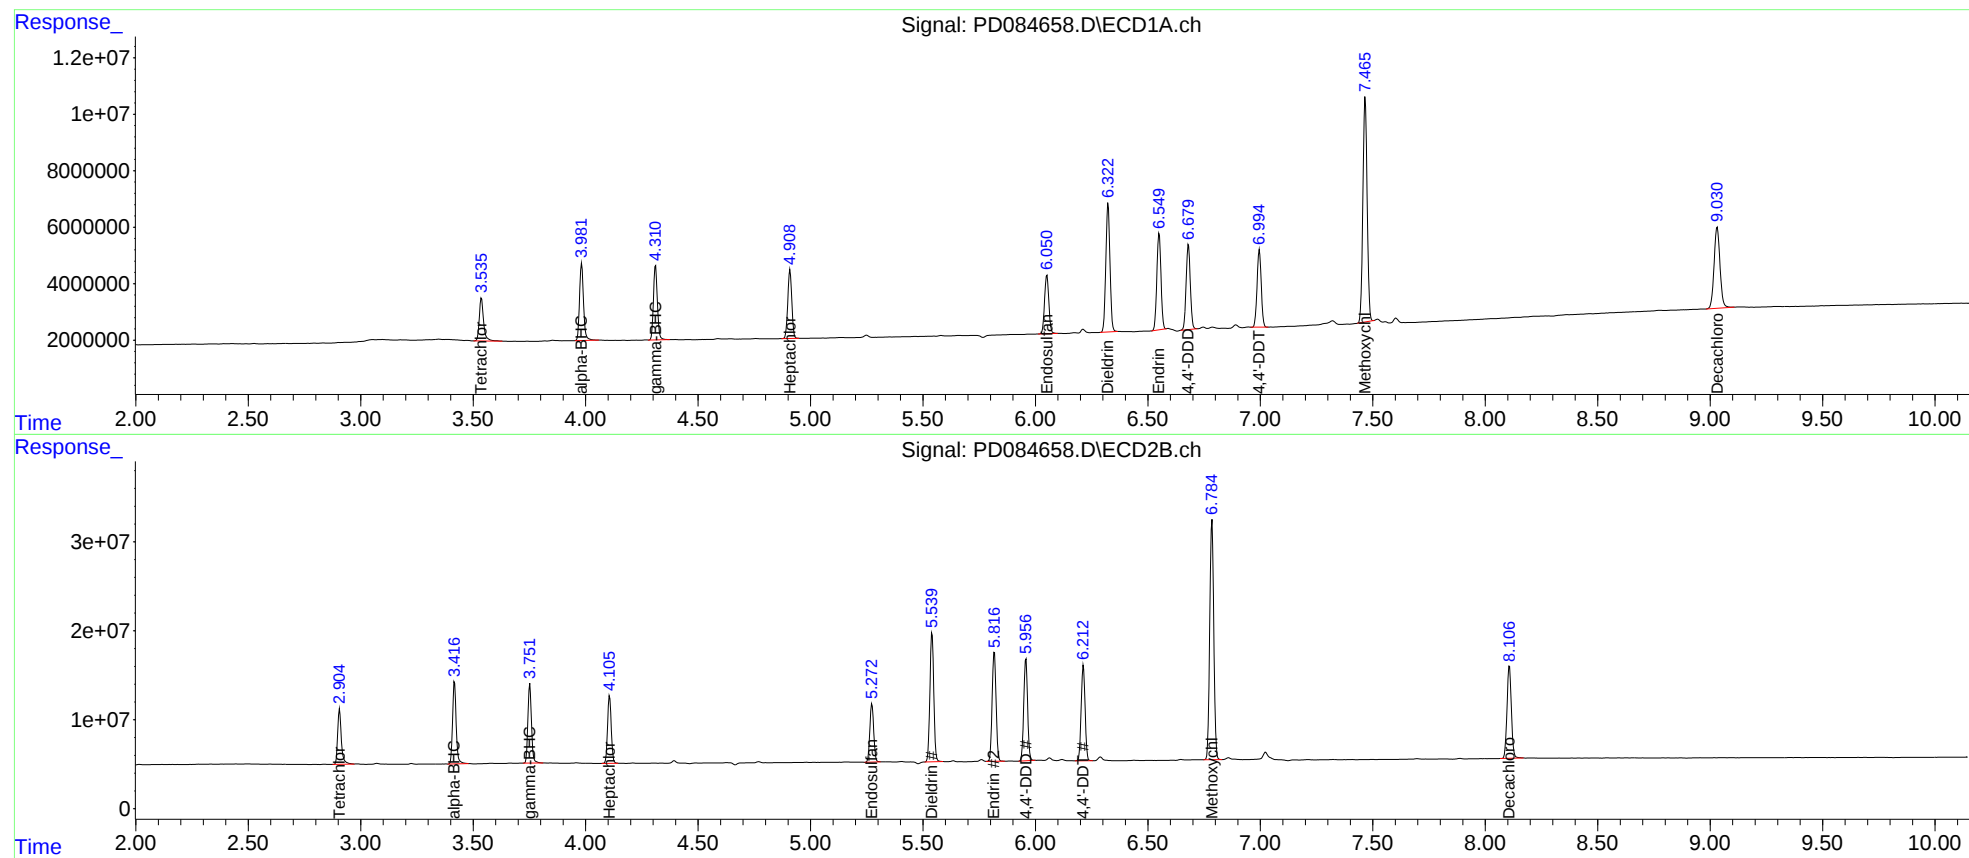

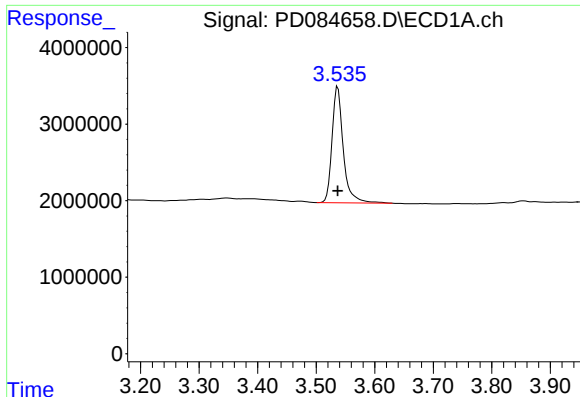


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 20264891
Conc: 20.00 ng/ml

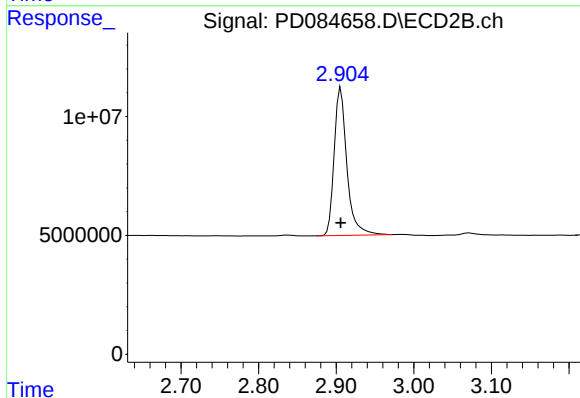


#1 Tetrachloro-m-xylene

R.T.: 2.906 min
Delta R.T.: 0.000 min
Response: 70845388
Conc: 20.00 ng/ml

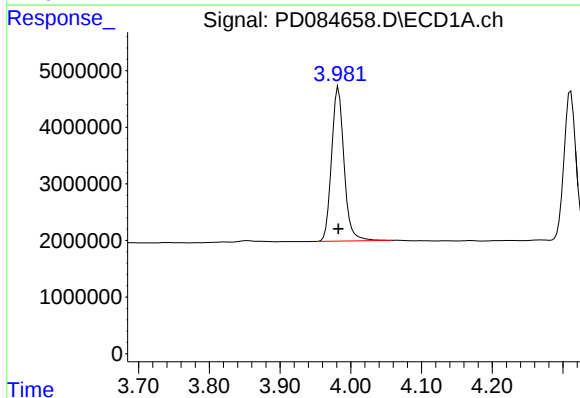


#2 alpha-BHC

R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 33294943
Conc: 20.00 ng/ml

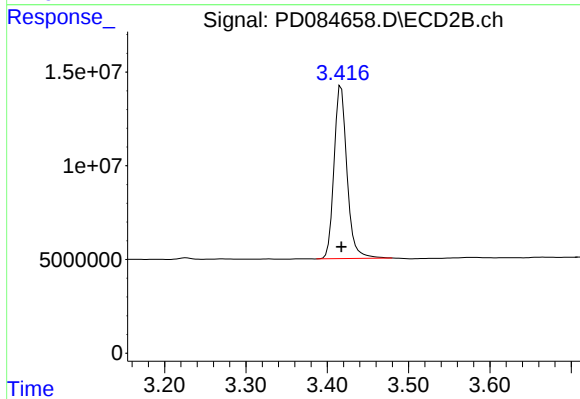


#2 alpha-BHC

R.T.: 3.417 min
Delta R.T.: 0.000 min
Response: 102094564
Conc: 20.00 ng/ml

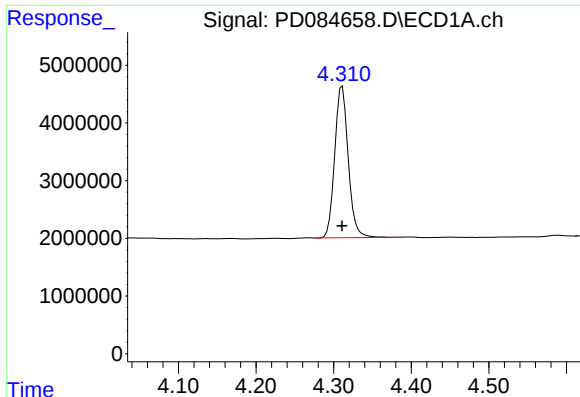


#3 gamma-BHC (Lindane)

R.T.: 4.311 min
Delta R.T.: 0.000 min
Response: 31815775
Conc: 20.00 ng/ml

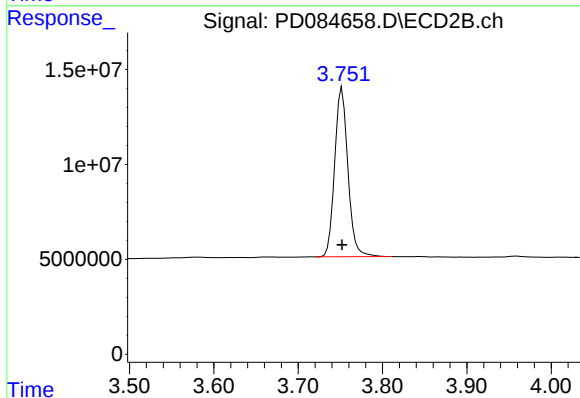


#3 gamma-BHC (Lindane)

R.T.: 3.752 min
Delta R.T.: 0.000 min
Response: 97284049
Conc: 20.00 ng/ml

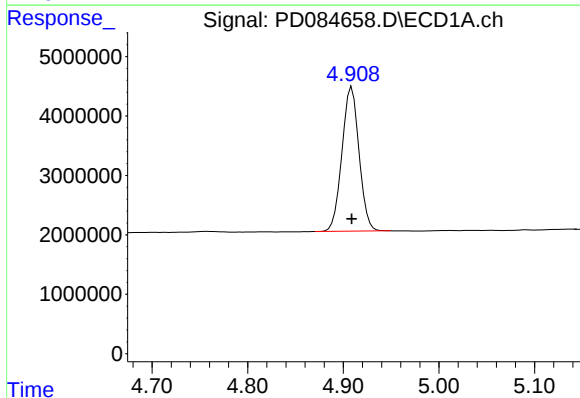


#4 Heptachlor

R.T.: 4.909 min
Delta R.T.: 0.000 min
Response: 30216696
Conc: 20.00 ng/ml

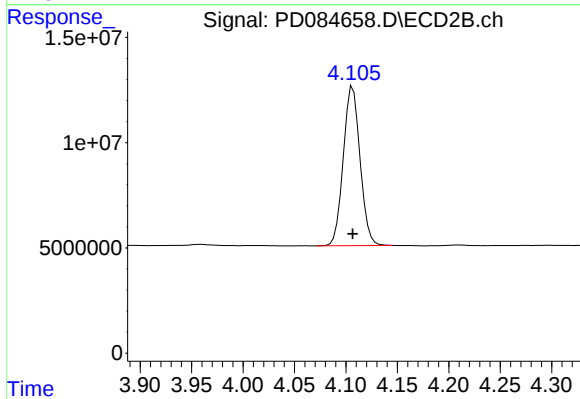


#4 Heptachlor

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 85840361
Conc: 20.00 ng/ml

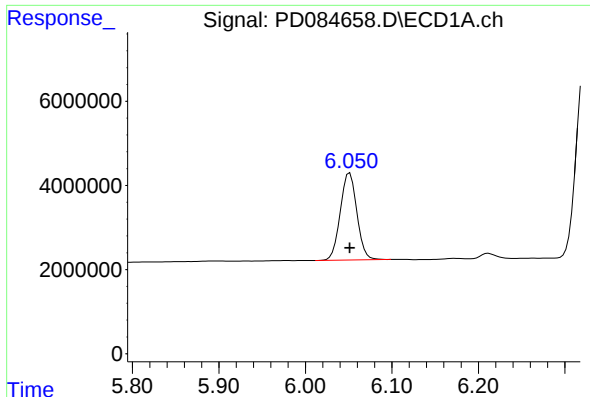


#9 Endosulfan I

R.T.: 6.051 min
Delta R.T.: 0.000 min
Response: 27458666
Conc: 20.00 ng/ml

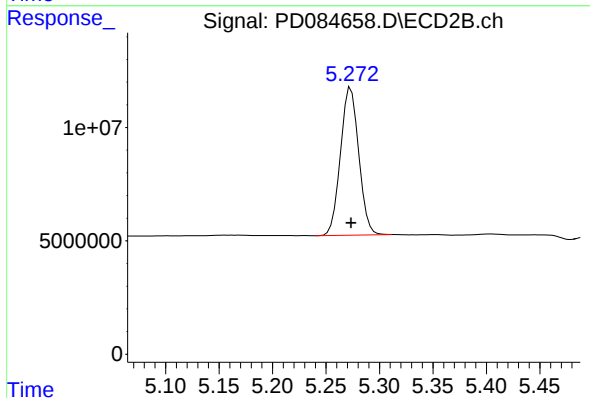


#9 Endosulfan I

R.T.: 5.273 min
Delta R.T.: 0.000 min
Response: 77570570
Conc: 20.00 ng/ml

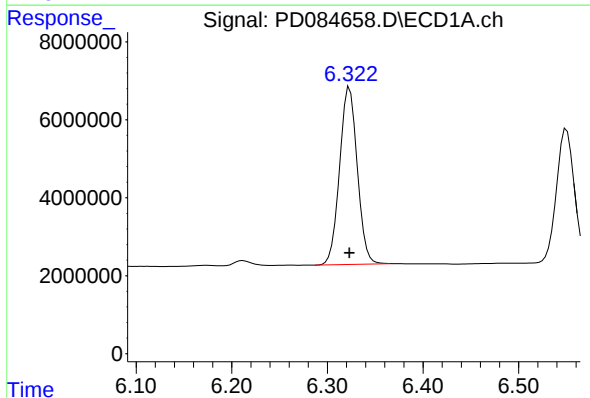


#13 Dieldrin

R.T.: 6.323 min
Delta R.T.: 0.000 min
Response: 58511743
Conc: 40.00 ng/ml

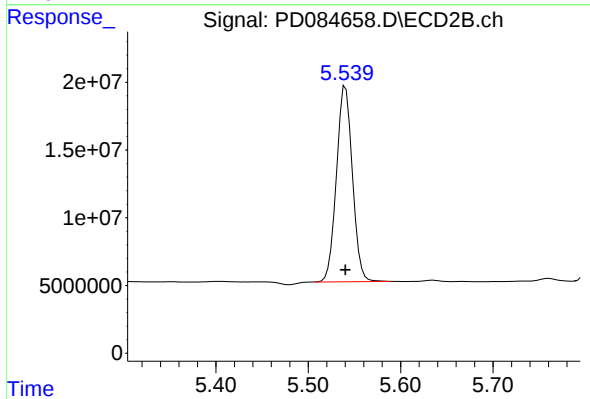


#13 Dieldrin

R.T.: 5.540 min
Delta R.T.: 0.000 min
Response: 173447779
Conc: 40.00 ng/ml

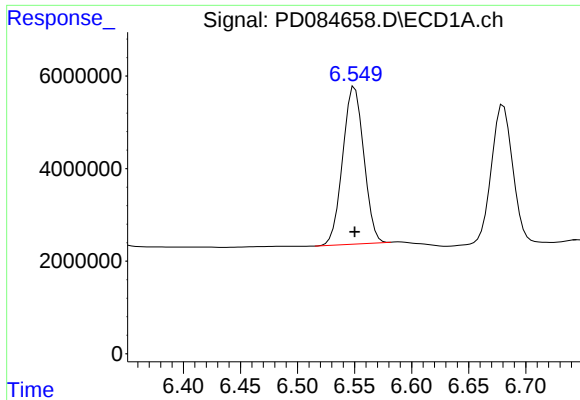


#14 Endrin

R.T.: 6.550 min
Delta R.T.: 0.000 min
Response: 43748411
Conc: 40.00 ng/ml

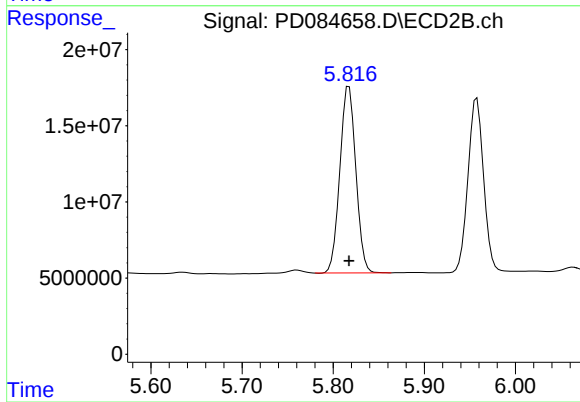


#14 Endrin

R.T.: 5.817 min
Delta R.T.: 0.000 min
Response: 149124389
Conc: 40.00 ng/ml

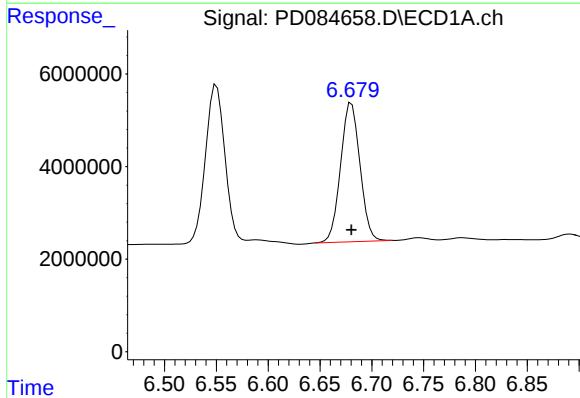


#16 4,4'-DDD

R.T.: 6.680 min
Delta R.T.: 0.000 min
Response: 39131439
Conc: 40.00 ng/ml

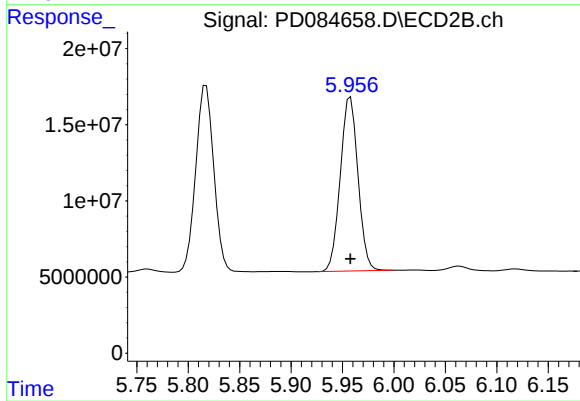


#16 4,4'-DDD

R.T.: 5.958 min
Delta R.T.: 0.000 min
Response: 136961806
Conc: 40.00 ng/ml

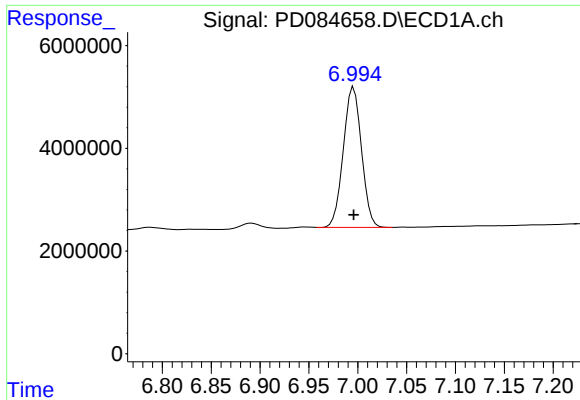


#17 4,4'-DDT

R.T.: 6.996 min
Delta R.T.: 0.000 min
Response: 35433115
Conc: 40.00 ng/ml

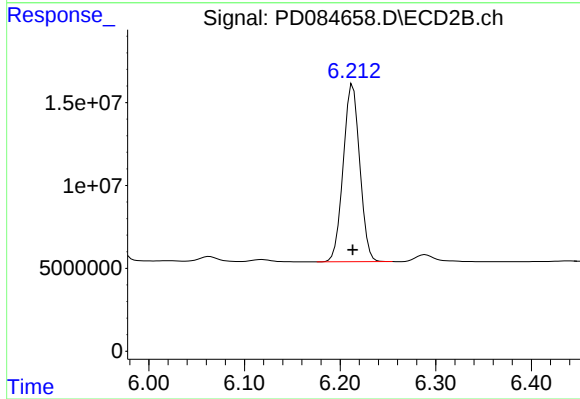


#17 4,4'-DDT

R.T.: 6.213 min
Delta R.T.: 0.000 min
Response: 129300035
Conc: 40.00 ng/ml

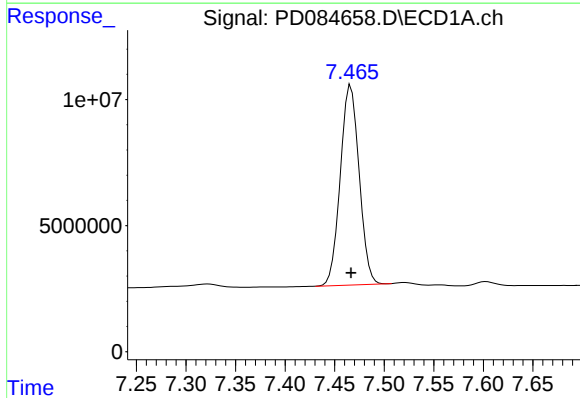


#20 Methoxychlor

R.T.: 7.466 min
Delta R.T.: 0.000 min
Response: 104989844
Conc: 200.00 ng/ml

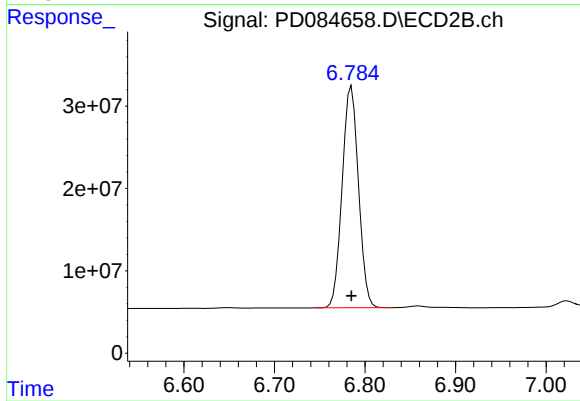


#20 Methoxychlor

R.T.: 6.785 min
Delta R.T.: 0.000 min
Response: 337270392
Conc: 200.00 ng/ml

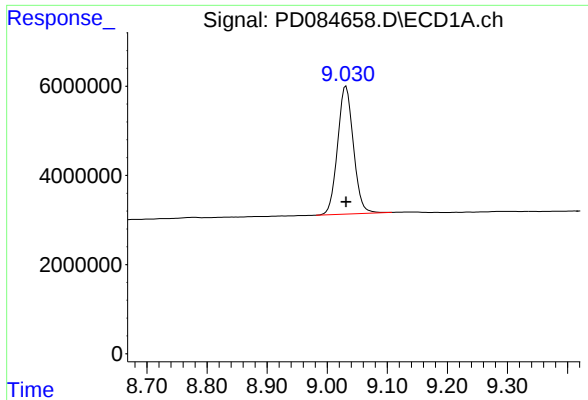

#27 Decachlorobiphenyl

R.T.: 9.031 min
Delta R.T.: 0.000 min
Response: 52465345
Conc: 40.00 ng/ml

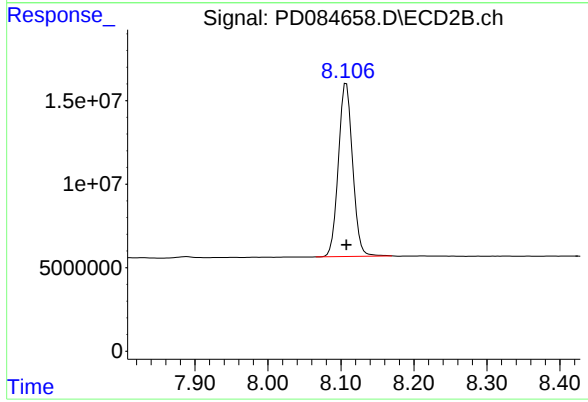

#27 Decachlorobiphenyl

R.T.: 8.107 min
Delta R.T.: 0.000 min
Response: 140383864
Conc: 40.00 ng/ml