

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082524\
 Data File : PD084660.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2024 02:07
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 05:30:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 23 05:28:46 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.906	40548042	142.3E6	40.018	40.168
27)	SA Decachlor...	9.031	8.107	103.0E6	269.7E6	78.518	76.859
Target Compounds							
2)	A alpha-BHC	3.983	3.417	72973146	207.0E6	43.834	40.553
3)	MA gamma-BHC...	4.312	3.752	69167770	195.7E6	43.480	40.225
4)	MA Heptachlor	4.909	4.107	64474614	171.9E6	42.675	40.054
9)	A Endosulfan I	6.051	5.273	56487693	152.6E6	41.144	39.358
13)	MA Dieldrin	6.324	5.540	125.0E6	345.0E6	85.436	79.562
14)	MA Endrin	6.551	5.817	99157472	298.5E6	90.662	80.056
16)	A 4,4'-DDD	6.681	5.958	83523339	272.4E6	85.377	79.545
17)	MA 4,4'-DDT	6.996	6.213	77760681	263.8E6	87.783	81.598
20)	A Methoxychlor	7.467	6.786	219.1E6	645.6E6	417.339	382.819


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082524\
Data File : PD084660.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2024 02:07
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 05:30:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Fri Aug 23 05:28:46 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

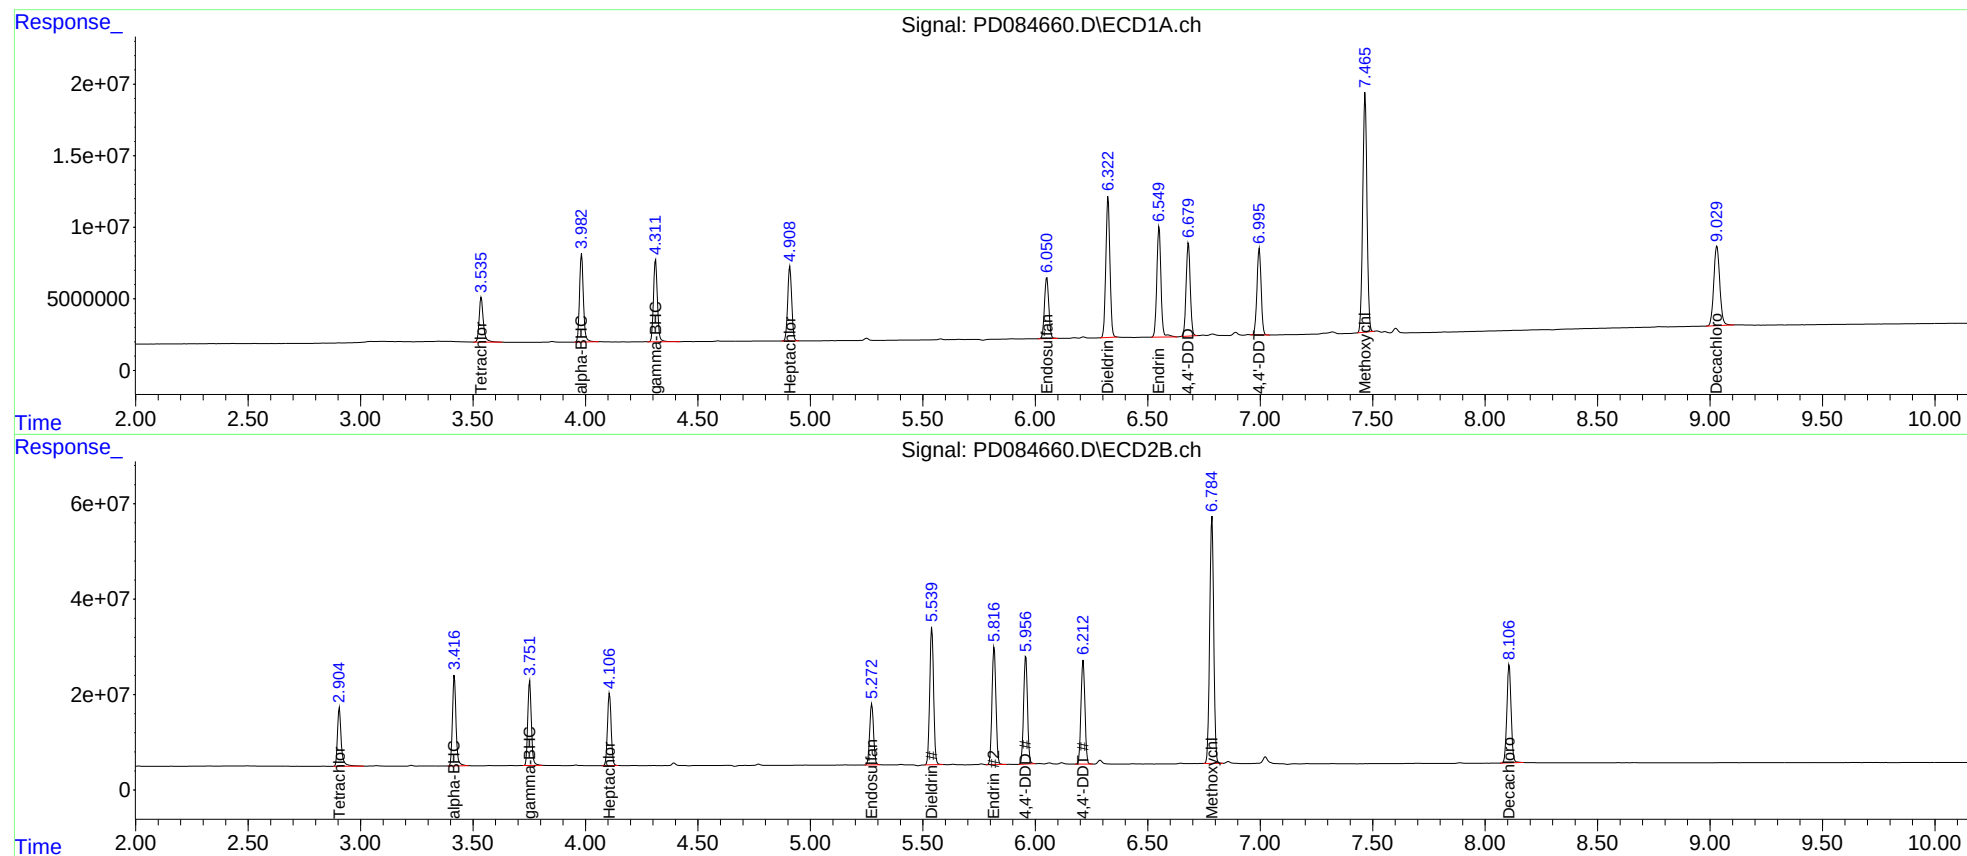

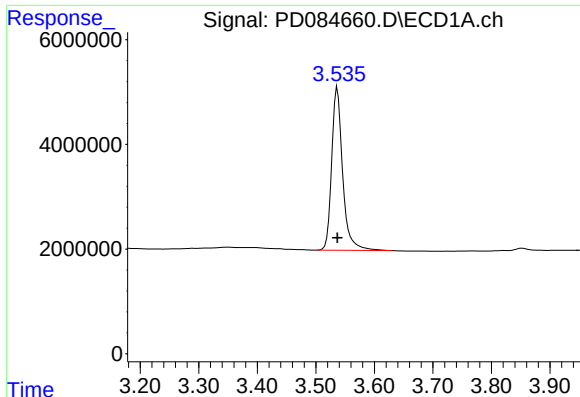


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 40548042
Conc: 40.02 ng/ml

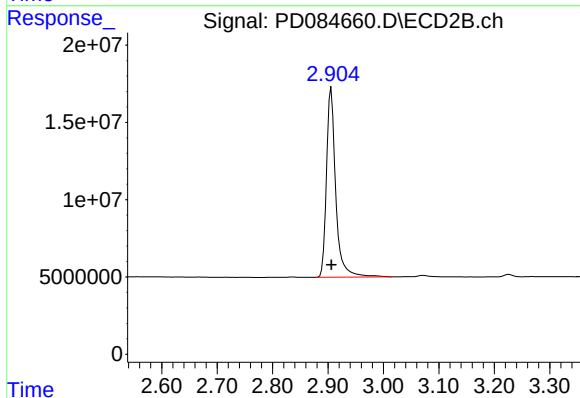


#1 Tetrachloro-m-xylene

R.T.: 2.906 min
Delta R.T.: 0.000 min
Response: 142287503
Conc: 40.17 ng/ml

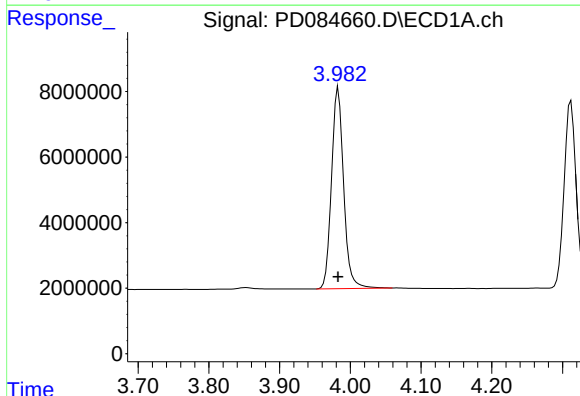


#2 alpha-BHC

R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 72973146
Conc: 43.83 ng/ml

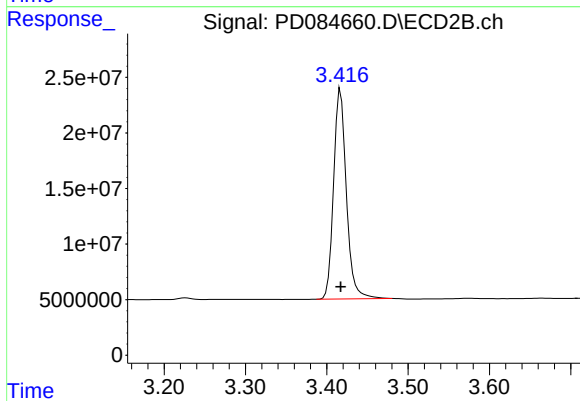


#2 alpha-BHC

R.T.: 3.417 min
Delta R.T.: 0.000 min
Response: 207014078
Conc: 40.55 ng/ml

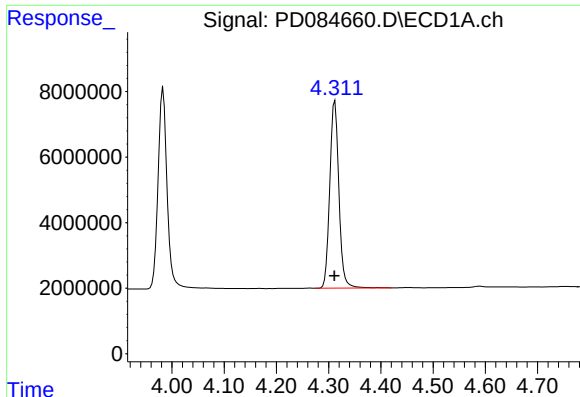


#3 gamma-BHC (Lindane)

R.T.: 4.312 min
Delta R.T.: 0.000 min
Response: 69167770
Conc: 43.48 ng/ml

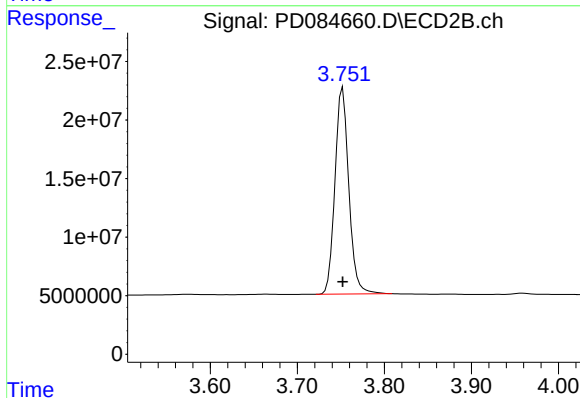


#3 gamma-BHC (Lindane)

R.T.: 3.752 min
Delta R.T.: 0.000 min
Response: 195661705
Conc: 40.22 ng/ml

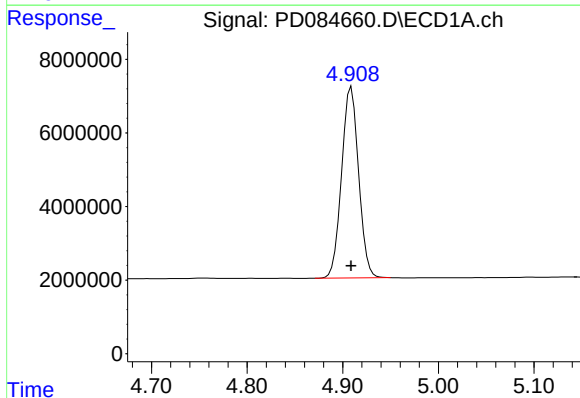


#4 Heptachlor

R.T.: 4.909 min
Delta R.T.: 0.000 min
Response: 64474614
Conc: 42.67 ng/ml

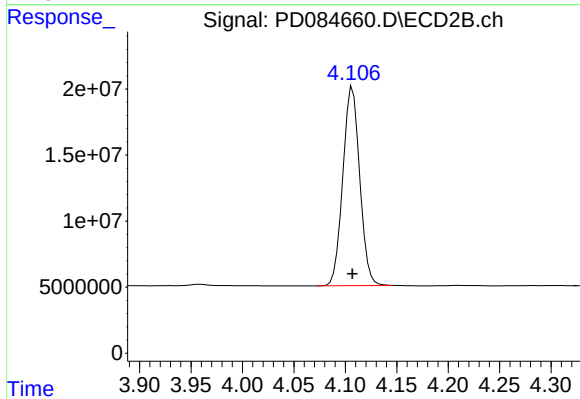


#4 Heptachlor

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 171910811
Conc: 40.05 ng/ml

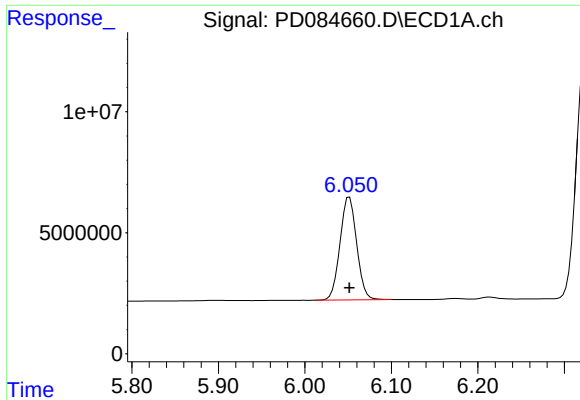


#9 Endosulfan I

R.T.: 6.051 min
Delta R.T.: 0.000 min
Response: 56487693
Conc: 41.14 ng/ml

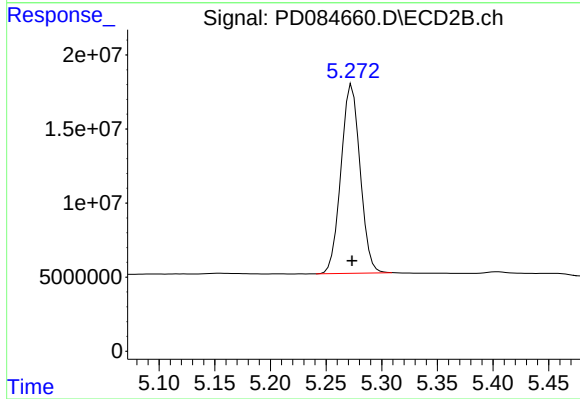


#9 Endosulfan I

R.T.: 5.273 min
Delta R.T.: 0.000 min
Response: 152649516
Conc: 39.36 ng/ml

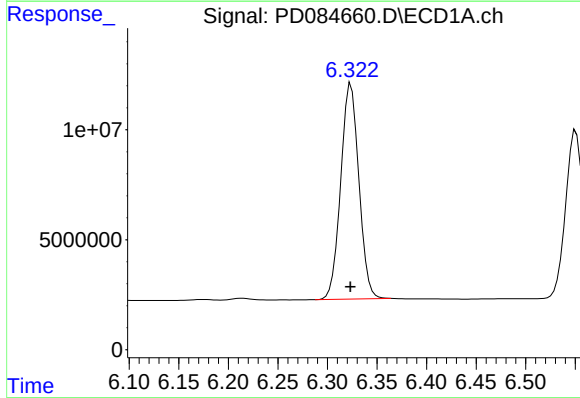


#13 Dieldrin

R.T.: 6.324 min
Delta R.T.: 0.000 min
Response: 124975946
Conc: 85.44 ng/ml

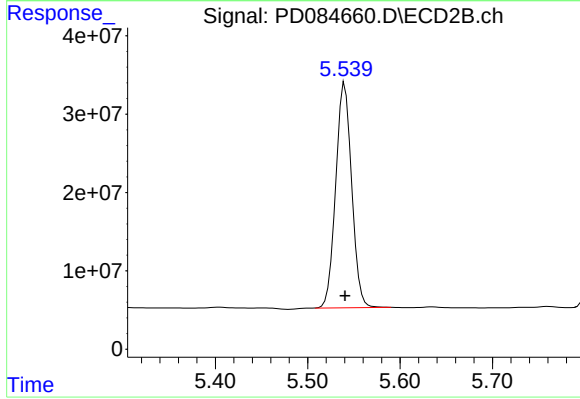


#13 Dieldrin

R.T.: 5.540 min
Delta R.T.: 0.000 min
Response: 344997345
Conc: 79.56 ng/ml

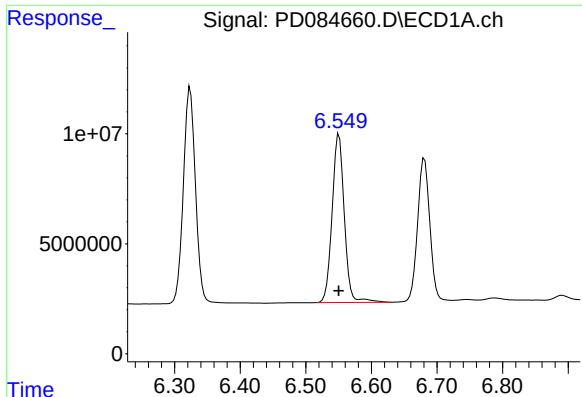


#14 Endrin

R.T.: 6.551 min
Delta R.T.: 0.000 min
Response: 99157472
Conc: 90.66 ng/ml

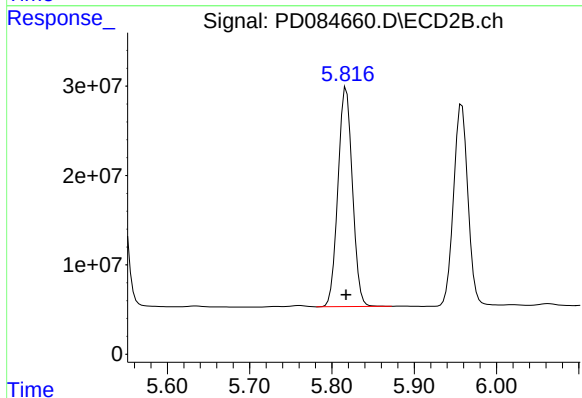


#14 Endrin

R.T.: 5.817 min
Delta R.T.: 0.000 min
Response: 298457269
Conc: 80.06 ng/ml

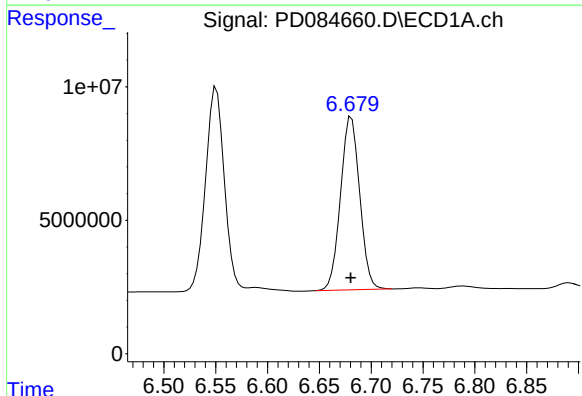


#16 4,4'-DDD

R.T.: 6.681 min
Delta R.T.: 0.000 min
Response: 83523339
Conc: 85.38 ng/ml

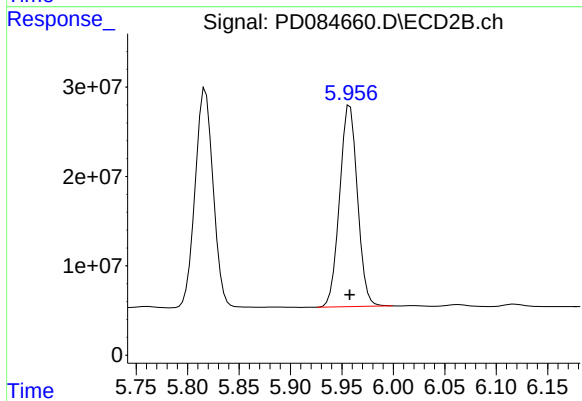


#16 4,4'-DDD

R.T.: 5.958 min
Delta R.T.: 0.000 min
Response: 272364705
Conc: 79.54 ng/ml

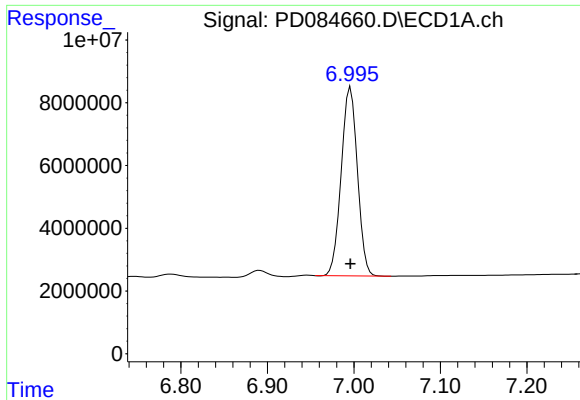


#17 4,4'-DDT

R.T.: 6.996 min
Delta R.T.: 0.000 min
Response: 77760681
Conc: 87.78 ng/ml

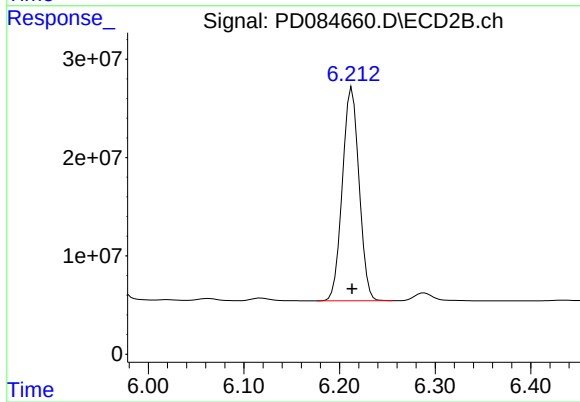


#17 4,4'-DDT

R.T.: 6.213 min
Delta R.T.: 0.000 min
Response: 263764219
Conc: 81.60 ng/ml

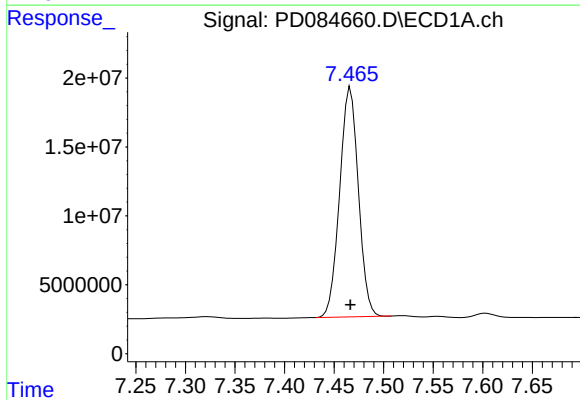


#20 Methoxychlor

R.T.: 7.467 min
Delta R.T.: 0.000 min
Response: 219081825
Conc: 417.34 ng/ml

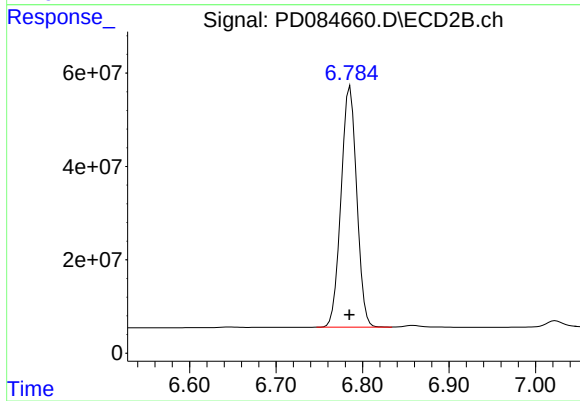


#20 Methoxychlor

R.T.: 6.786 min
Delta R.T.: 0.000 min
Response: 645567396
Conc: 382.82 ng/ml

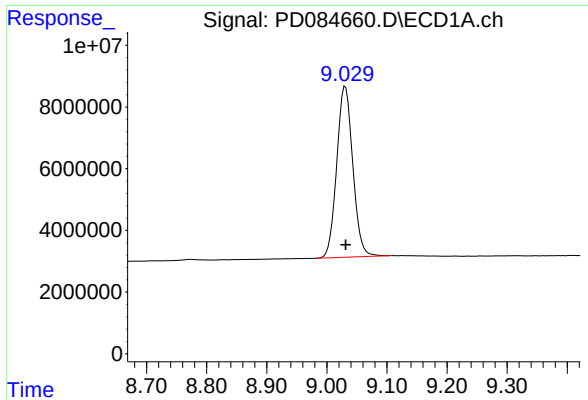

#27 Decachlorobiphenyl

R.T.: 9.031 min
Delta R.T.: 0.000 min
Response: 102987373
Conc: 78.52 ng/ml

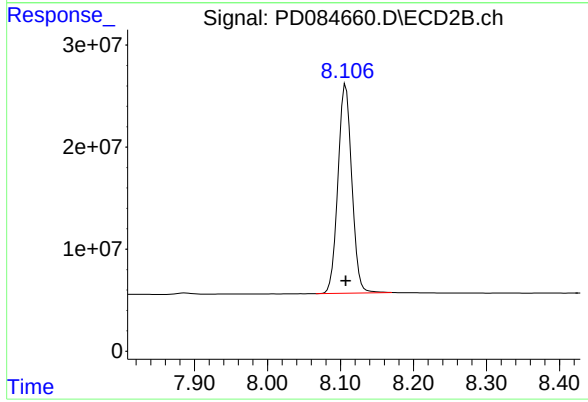

#27 Decachlorobiphenyl

R.T.: 8.107 min
Delta R.T.: 0.000 min
Response: 269745074
Conc: 76.86 ng/ml