

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082524\
 Data File : PD084661.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2024 02:21
 Operator : AR\AJ
 Sample : INDB401
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 02:23:58 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:21:37 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.906	40678165	141.9E6	39.371	38.677
27)	SA Decachlor...	9.031	8.107	103.0E6	269.3E6	78.466	75.991
Target Compounds							
5)	MB Aldrin	5.250	4.393	65812744	177.7E6	41.668	39.464
6)	B beta-BHC	4.494	4.045	28978511	84578482	39.754	38.252
7)	B delta-BHC	4.741	4.282	68641223	199.1E6	42.722	39.771
8)	B Heptachlo...	5.669	4.897	60261186	165.8E6	41.091	38.705
10)	B trans-Chl...	5.923	5.151	57460775	161.4E6	41.134	38.847
11)	B cis-Chlor...	6.004	5.216	59939479	164.4E6	40.800	38.725
12)	B 4,4'-DDE	6.173	5.401	109.2E6	312.6E6	88.900	78.831
15)	B Endosulfa...	6.761	6.109	104.2E6	291.2E6	82.036	77.462
18)	B Endrin al...	6.890	6.288	73341049	221.5E6	81.643	77.866
19)	B Endosulfa...	7.124	6.512	95012550	276.9E6	83.086	76.878
21)	B Endrin ke...	7.603	7.023	101.1E6	332.7E6	82.890	76.008


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082524\
Data File : PD084661.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2024 02:21
Operator : AR\AJ
Sample : INDB401
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 02:23:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:21:37 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

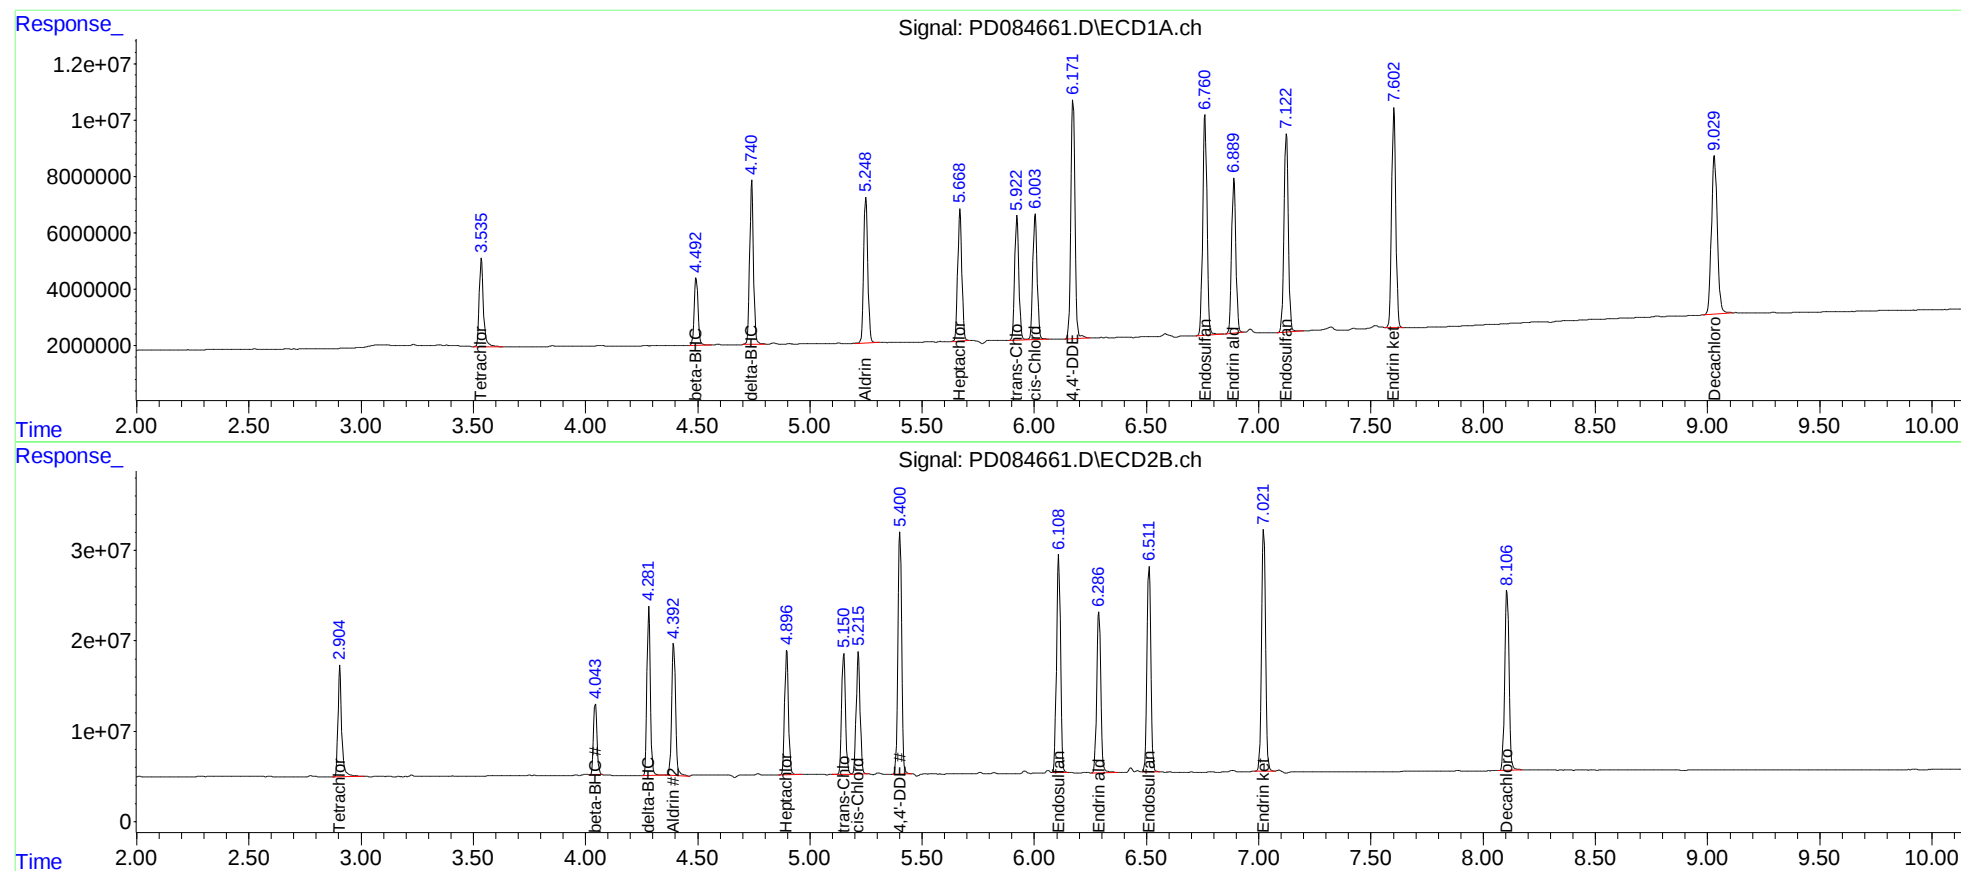

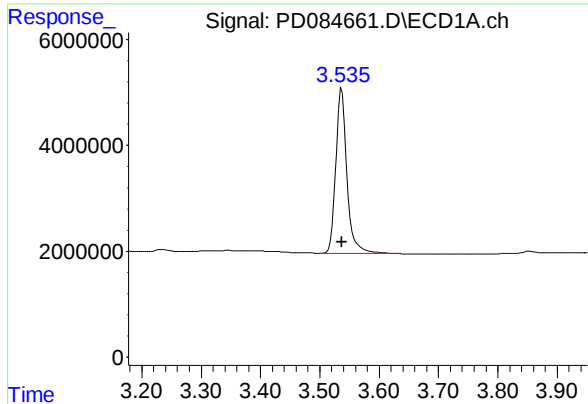


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 40678165
Conc: 39.37 ng/ml

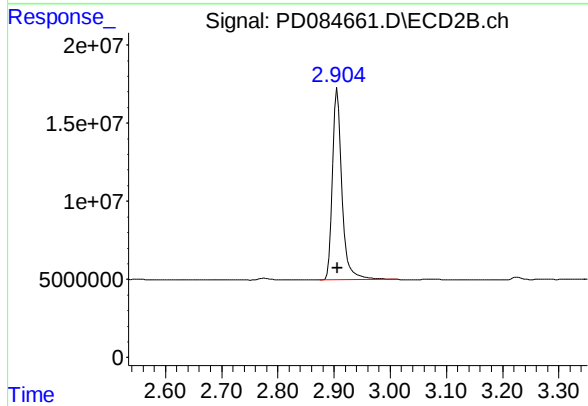


#1 Tetrachloro-m-xylene

R.T.: 2.906 min
Delta R.T.: 0.000 min
Response: 141893075
Conc: 38.68 ng/ml

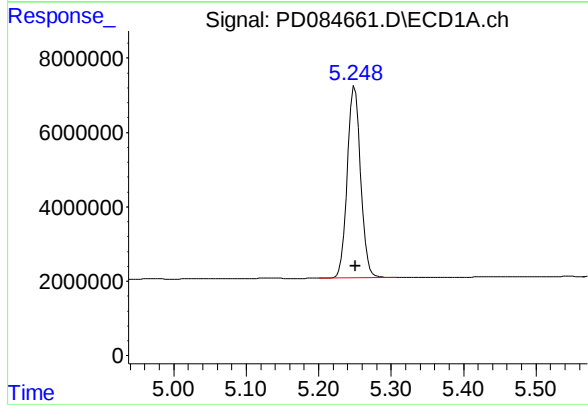


#5 Aldrin

R.T.: 5.250 min
Delta R.T.: 0.000 min
Response: 65812744
Conc: 41.67 ng/ml

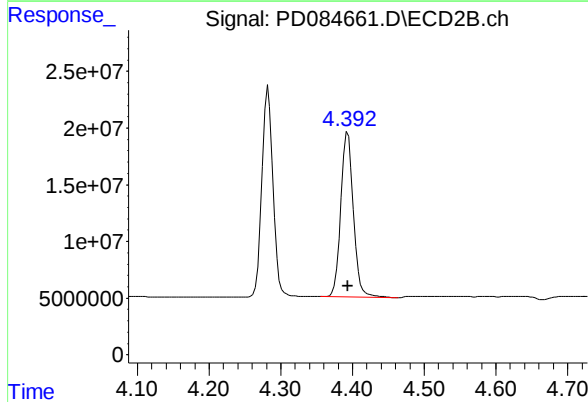


#5 Aldrin

R.T.: 4.393 min
Delta R.T.: 0.000 min
Response: 177682750
Conc: 39.46 ng/ml

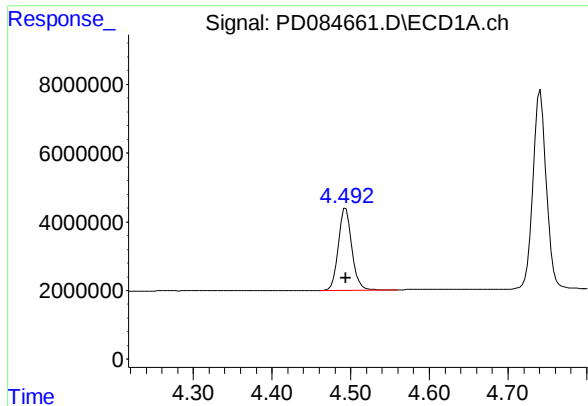


#6 beta-BHC

R.T.: 4.494 min
Delta R.T.: 0.000 min
Response: 28978511
Conc: 39.75 ng/ml

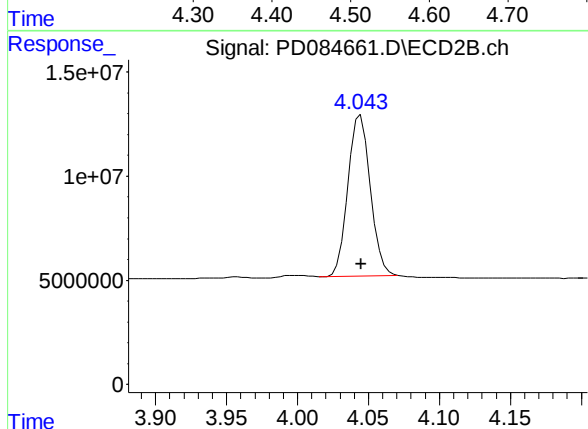


#6 beta-BHC

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 84578482
Conc: 38.25 ng/ml

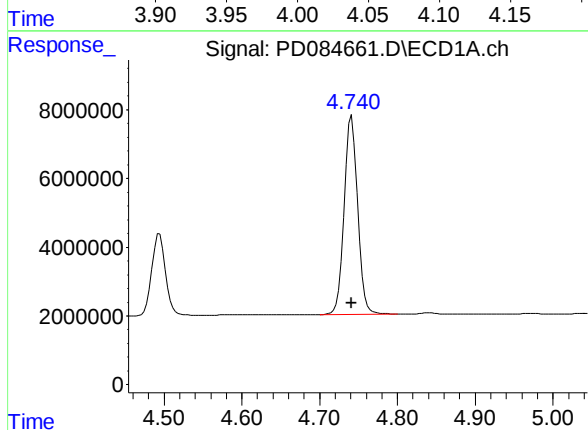


#7 delta-BHC

R.T.: 4.741 min
Delta R.T.: 0.000 min
Response: 68641223
Conc: 42.72 ng/ml

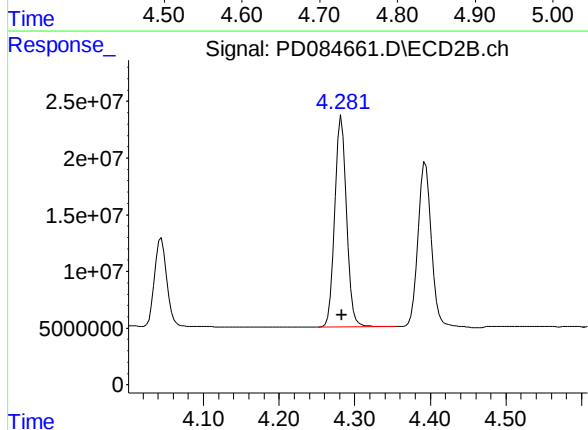


#7 delta-BHC

R.T.: 4.282 min
Delta R.T.: 0.000 min
Response: 199081595
Conc: 39.77 ng/ml

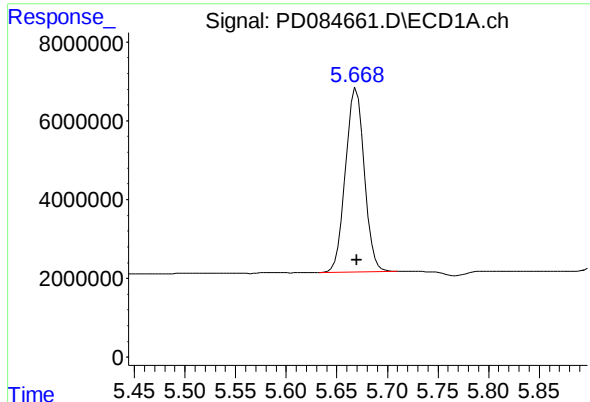


#8 Heptachlor epoxide

R.T.: 5.669 min
Delta R.T.: 0.000 min
Response: 60261186
Conc: 41.09 ng/ml

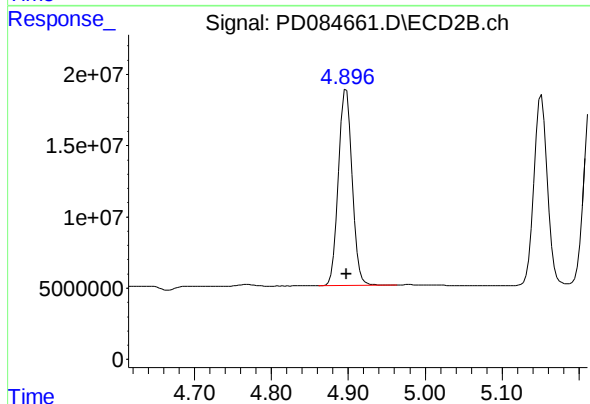


#8 Heptachlor epoxide

R.T.: 4.897 min
Delta R.T.: 0.000 min
Response: 165848403
Conc: 38.71 ng/ml

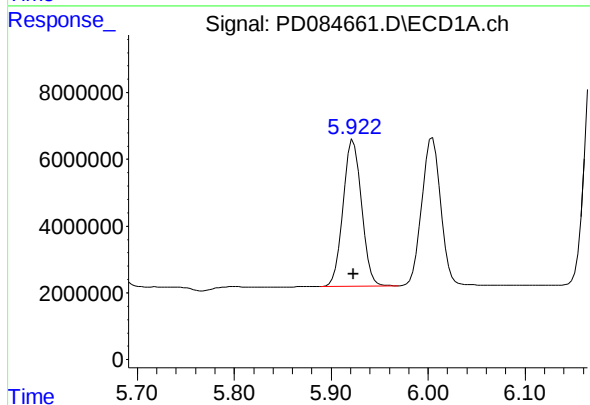


#10 trans-Chlordane

R.T.: 5.923 min
Delta R.T.: 0.000 min
Response: 57460775
Conc: 41.13 ng/ml

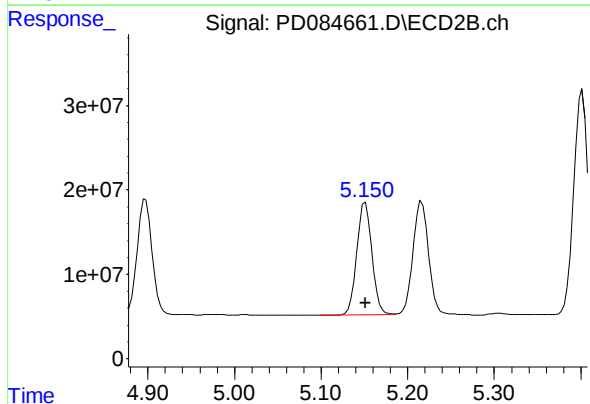


#10 trans-Chlordane

R.T.: 5.151 min
Delta R.T.: 0.000 min
Response: 161445243
Conc: 38.85 ng/ml

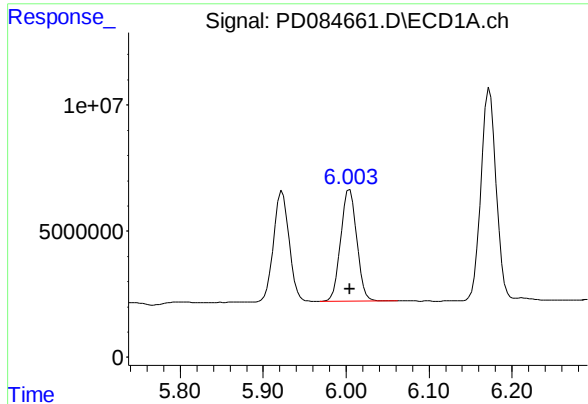


#11 cis-Chlordane

R.T.: 6.004 min
Delta R.T.: 0.000 min
Response: 59939479
Conc: 40.80 ng/ml

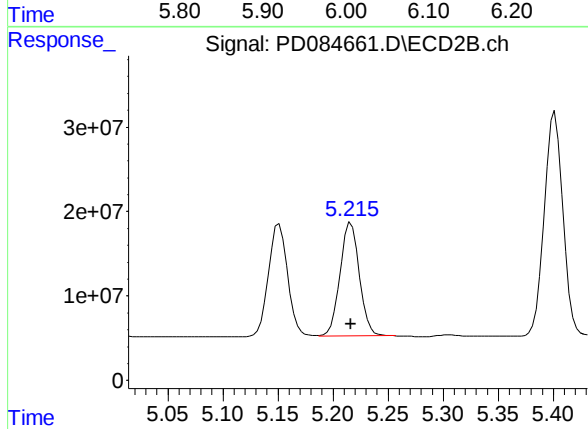


#11 cis-Chlordane

R.T.: 5.216 min
Delta R.T.: 0.000 min
Response: 164367947
Conc: 38.73 ng/ml

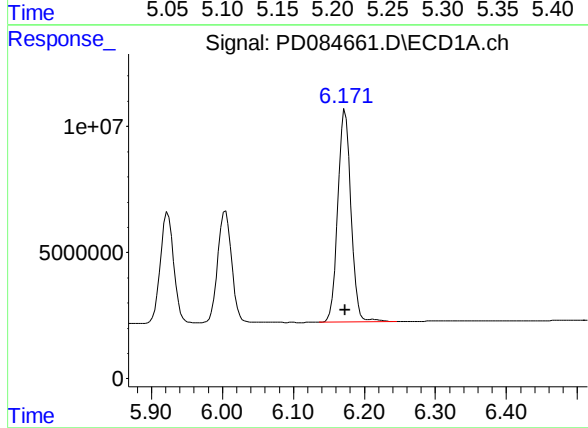


#12 4,4'-DDE

R.T.: 6.173 min
Delta R.T.: 0.000 min
Response: 109165182
Conc: 88.90 ng/ml

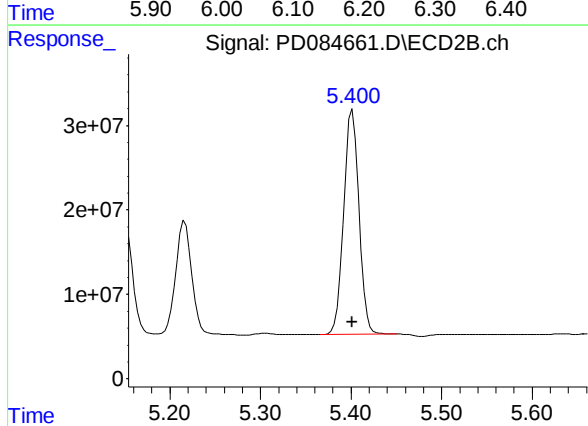


#12 4,4'-DDE

R.T.: 5.401 min
Delta R.T.: 0.000 min
Response: 312621859
Conc: 78.83 ng/ml

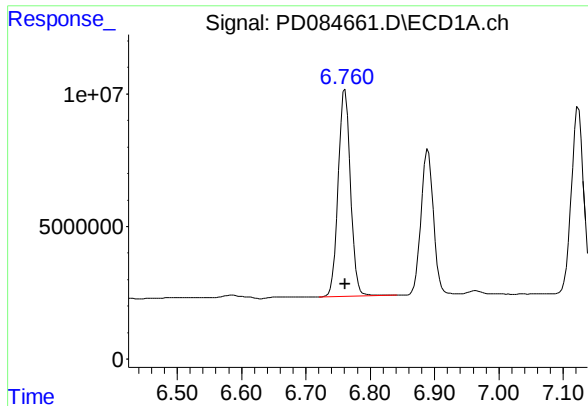


#15 Endosulfan II

R.T.: 6.761 min
Delta R.T.: 0.000 min
Response: 104186459
Conc: 82.04 ng/ml

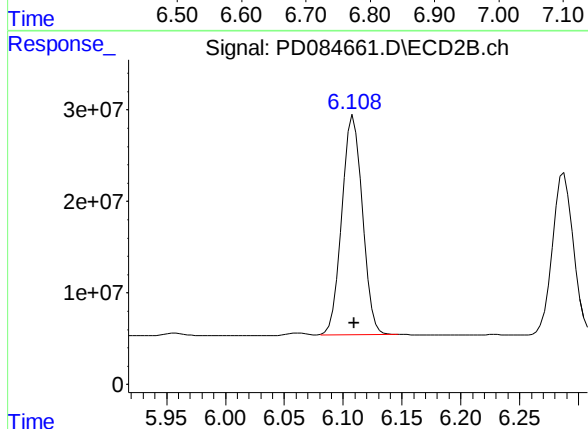


#15 Endosulfan II

R.T.: 6.109 min
Delta R.T.: 0.000 min
Response: 291238796
Conc: 77.46 ng/ml

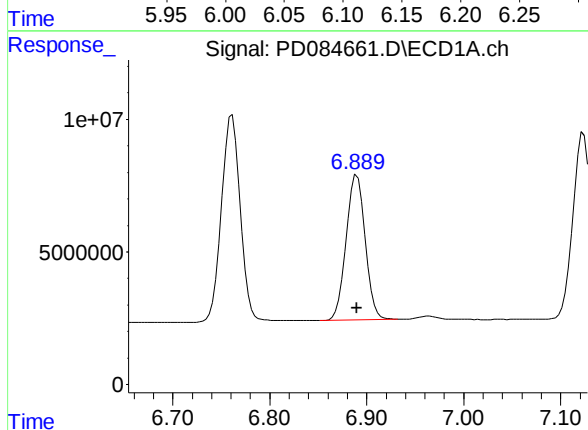


#18 Endrin aldehyde

R.T.: 6.890 min
Delta R.T.: 0.000 min
Response: 73341049
Conc: 81.64 ng/ml

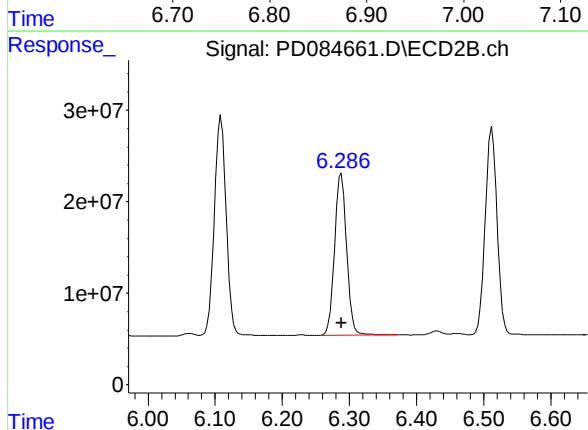


#18 Endrin aldehyde

R.T.: 6.288 min
Delta R.T.: 0.000 min
Response: 221501498
Conc: 77.87 ng/ml

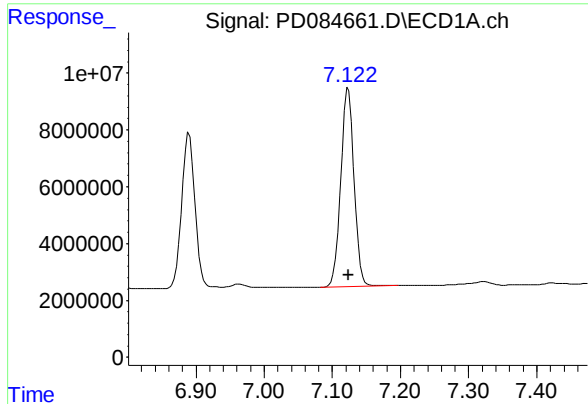


#19 Endosulfan Sulfate

R.T.: 7.124 min
Delta R.T.: 0.000 min
Response: 95012550
Conc: 83.09 ng/ml

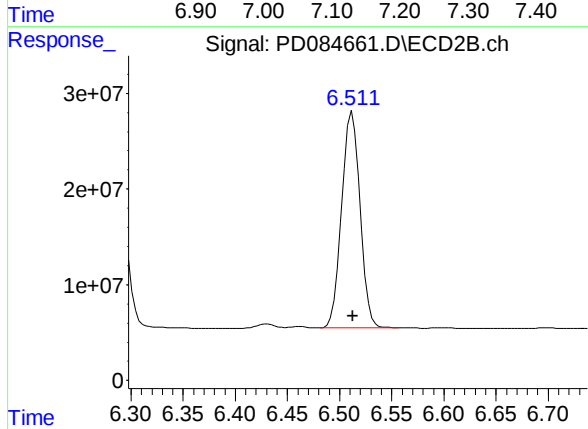


#19 Endosulfan Sulfate

R.T.: 6.512 min
Delta R.T.: 0.000 min
Response: 276948326
Conc: 76.88 ng/ml

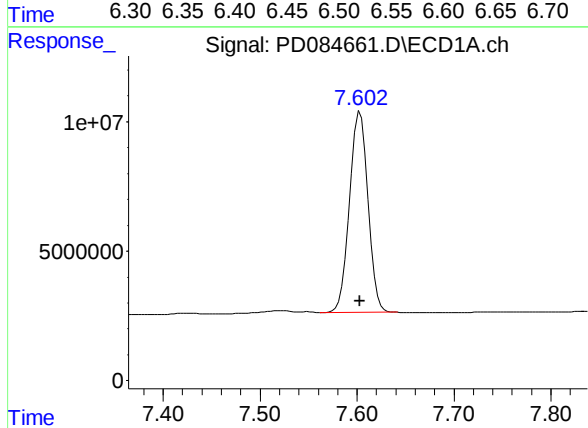


#21 Endrin ketone

R.T.: 7.603 min
Delta R.T.: 0.000 min
Response: 101082134
Conc: 82.89 ng/ml

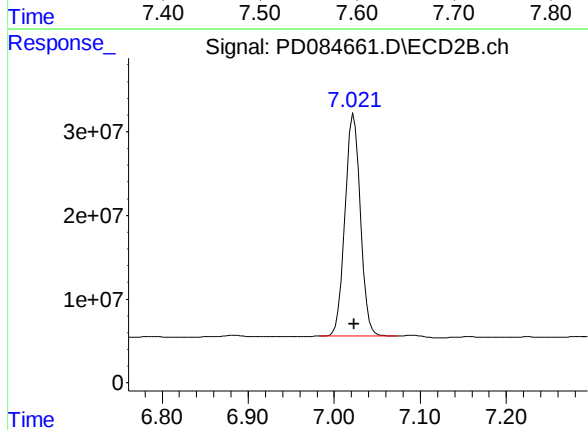


#21 Endrin ketone

R.T.: 7.023 min
Delta R.T.: 0.000 min
Response: 332695888
Conc: 76.01 ng/ml

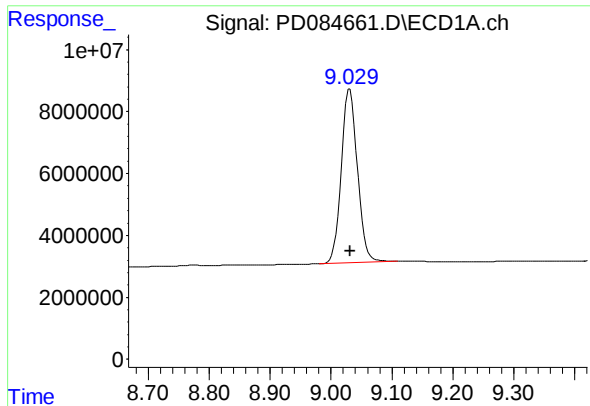

#27 Decachlorobiphenyl

R.T.: 9.031 min
Delta R.T.: 0.000 min
Response: 102959007
Conc: 78.47 ng/ml

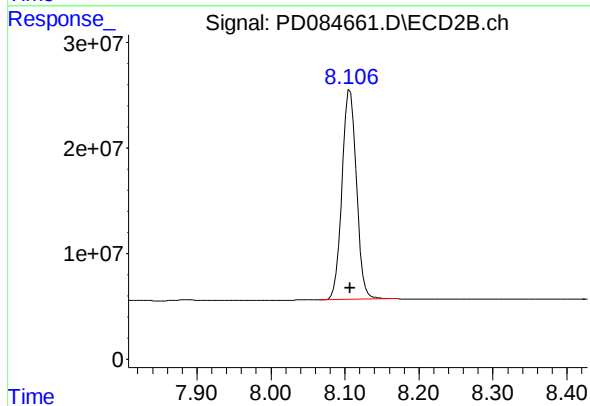

#27 Decachlorobiphenyl

R.T.: 8.107 min
Delta R.T.: 0.000 min
Response: 269322325
Conc: 75.99 ng/ml