

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082524\
 Data File : PD084662.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2024 02:34
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 05:30:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 23 05:28:46 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.906	82217592	280.6E6	81.143	79.209
27)	SA Decachlor...	9.032	8.107	207.3E6	528.6E6	158.010	150.611
Target Compounds							
2)	A alpha-BHC	3.983	3.417	162.7E6	422.0E6	97.735	82.665
3)	MA gamma-BHC...	4.312	3.752	151.9E6	395.3E6	95.473	81.273
4)	MA Heptachlor	4.909	4.107	140.0E6	346.1E6	92.683	80.649
9)	A Endosulfan I	6.052	5.273	118.6E6	302.8E6	86.364	78.076
13)	MA Dieldrin	6.324	5.540	271.9E6	690.0E6	185.896	159.123
14)	MA Endrin	6.550	5.818	215.3E6	596.2E6	196.884	159.930
16)	A 4,4'-DDD	6.681	5.958	182.6E6	544.3E6	186.679	158.959
17)	MA 4,4'-DDT	6.996	6.213	174.2E6	538.3E6	196.644	166.533
20)	A Methoxychlor	7.466	6.786	461.8E6	1223.7E6	879.666	725.637


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082524\
Data File : PD084662.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2024 02:34
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 05:30:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Fri Aug 23 05:28:46 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

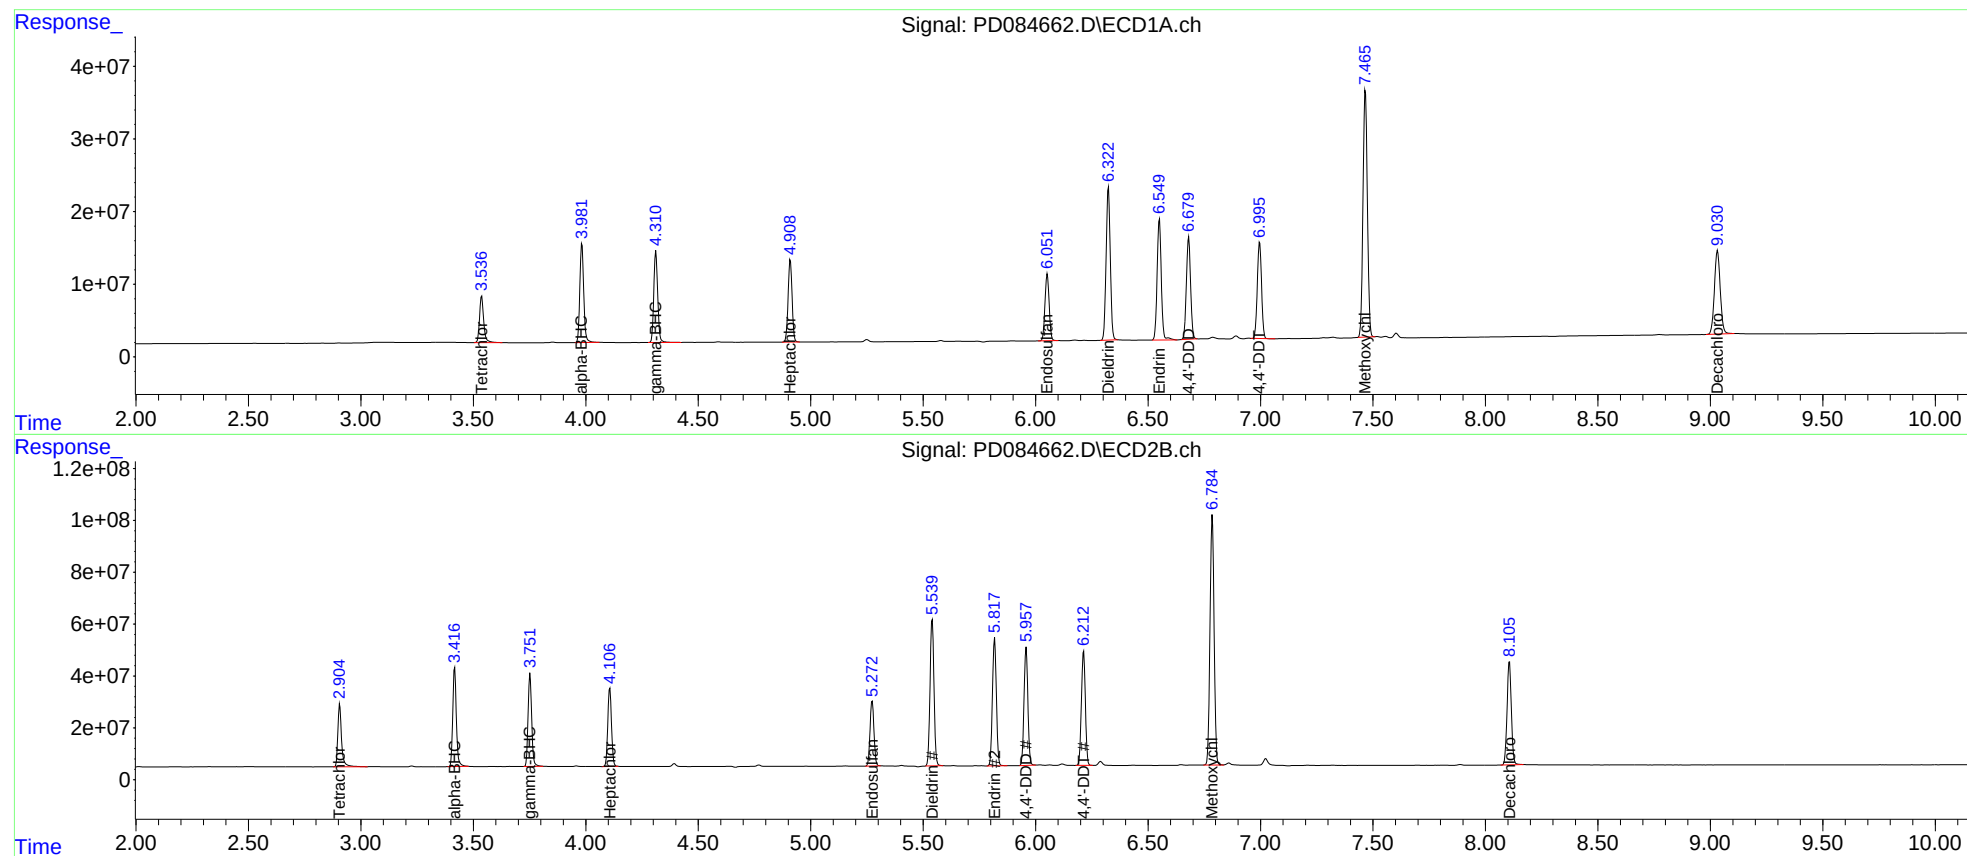

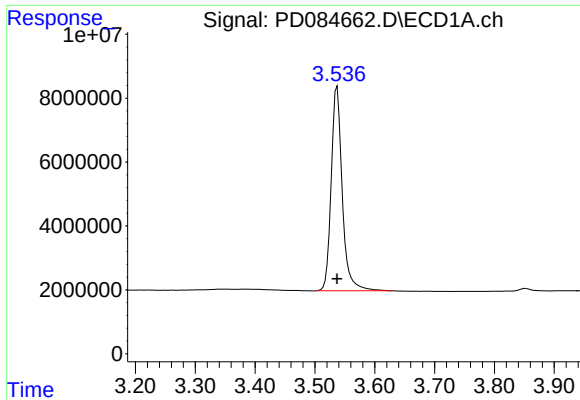


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 82217592
Conc: 81.14 ng/ml

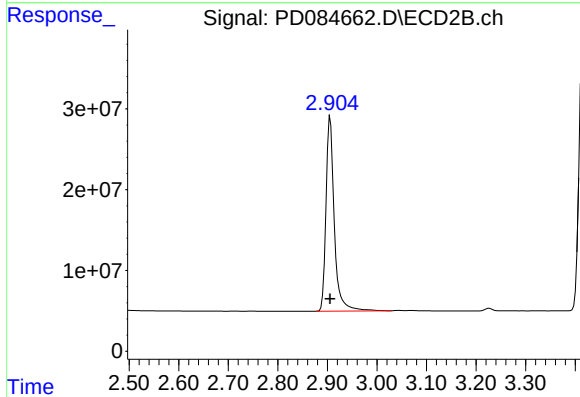


#1 Tetrachloro-m-xylene

R.T.: 2.906 min
Delta R.T.: 0.000 min
Response: 280580861
Conc: 79.21 ng/ml

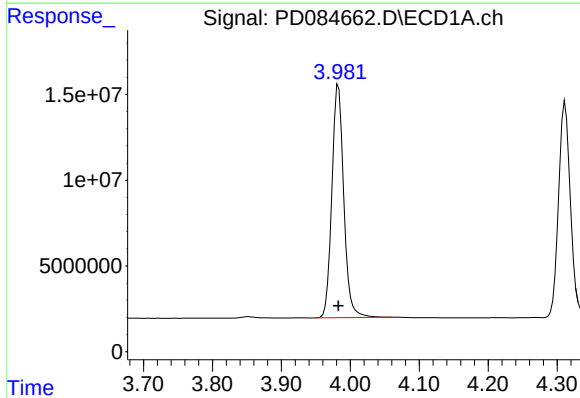


#2 alpha-BHC

R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 162703408
Conc: 97.73 ng/ml

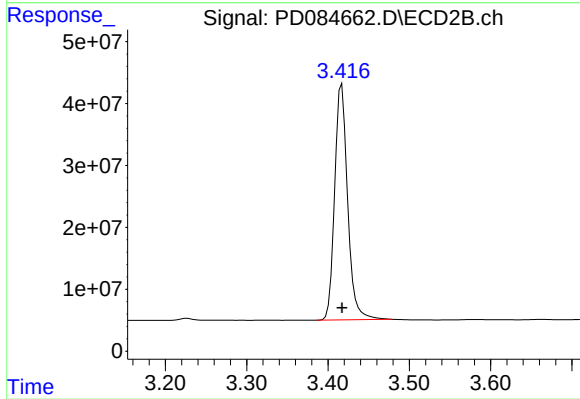

#2 alpha-BHC

R.T.: 3.417 min
Delta R.T.: 0.000 min
Response: 421982144
Conc: 82.66 ng/ml

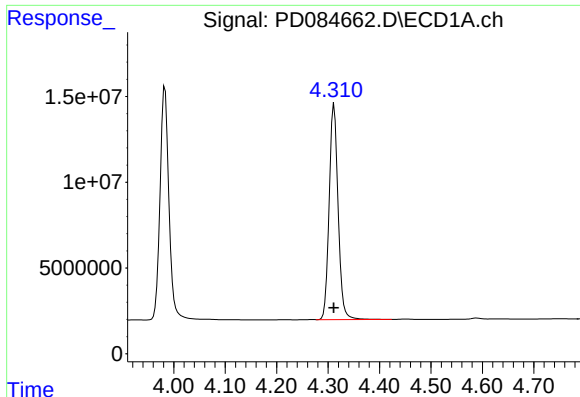


#3 gamma-BHC (Lindane)

R.T.: 4.312 min

Delta R.T.: 0.000 min

Response: 151877612

Conc: 95.47 ng/ml

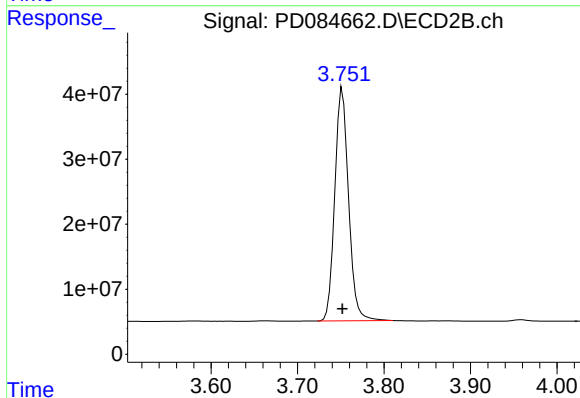


#3 gamma-BHC (Lindane)

R.T.: 3.752 min

Delta R.T.: 0.000 min

Response: 395328559

Conc: 81.27 ng/ml

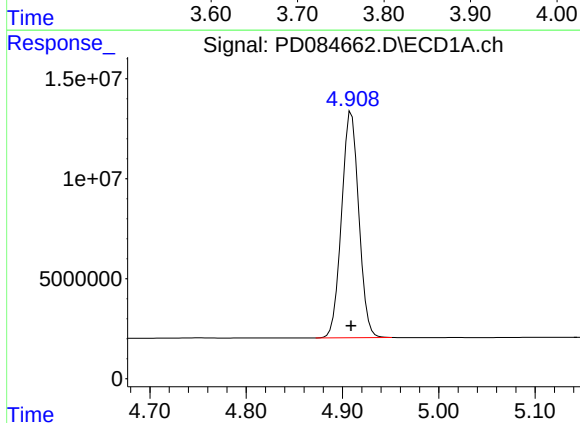


#4 Heptachlor

R.T.: 4.909 min

Delta R.T.: 0.000 min

Response: 140028283

Conc: 92.68 ng/ml

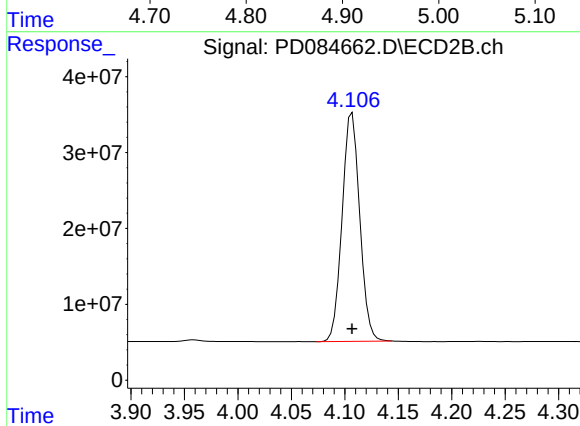


#4 Heptachlor

R.T.: 4.107 min

Delta R.T.: 0.000 min


Response: 346145665

Conc: 80.65 ng/ml

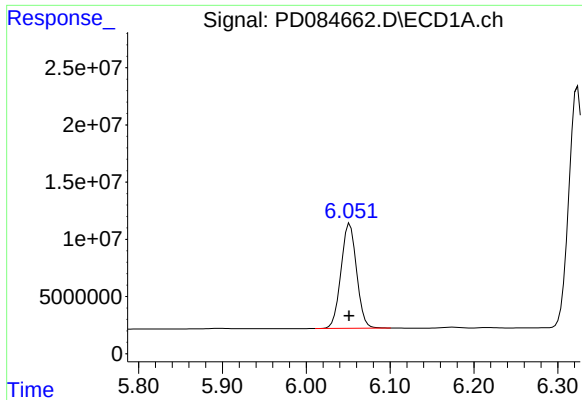


#9 Endosulfan I

R.T.: 6.052 min
Delta R.T.: 0.000 min
Response: 118572480
Conc: 86.36 ng/ml

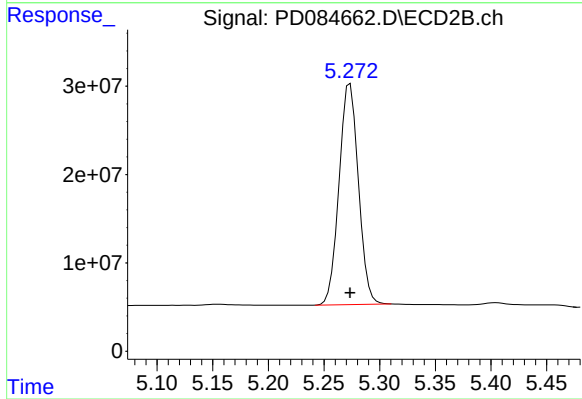


#9 Endosulfan I

R.T.: 5.273 min
Delta R.T.: 0.000 min
Response: 302819182
Conc: 78.08 ng/ml

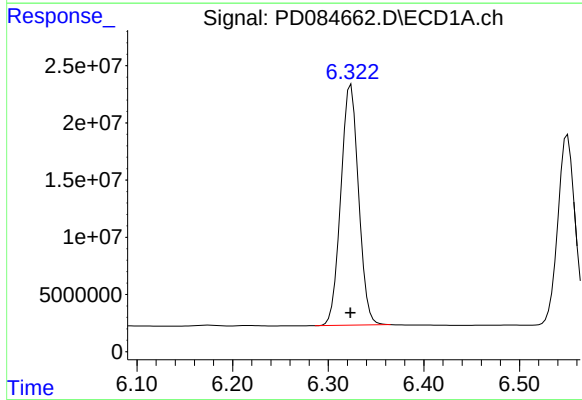


#13 Dieldrin

R.T.: 6.324 min
Delta R.T.: 0.000 min
Response: 271926959
Conc: 185.90 ng/ml

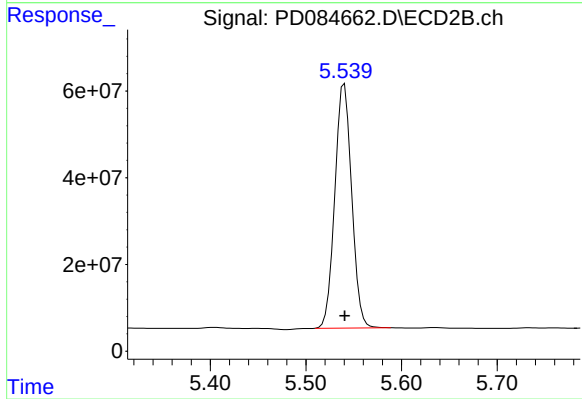


#13 Dieldrin

R.T.: 5.540 min
Delta R.T.: 0.000 min
Response: 689987164
Conc: 159.12 ng/ml

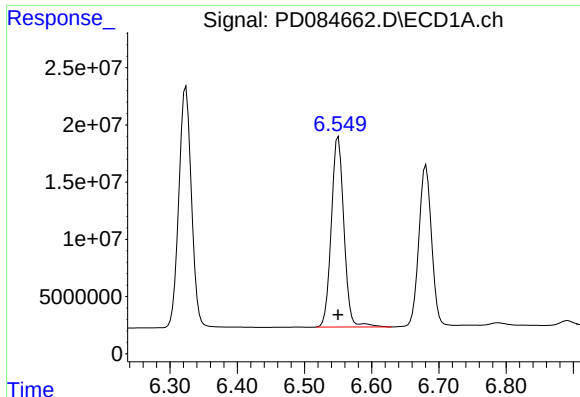


#14 Endrin

R.T.: 6.550 min
Delta R.T.: 0.000 min
Response: 215334574
Conc: 196.88 ng/ml

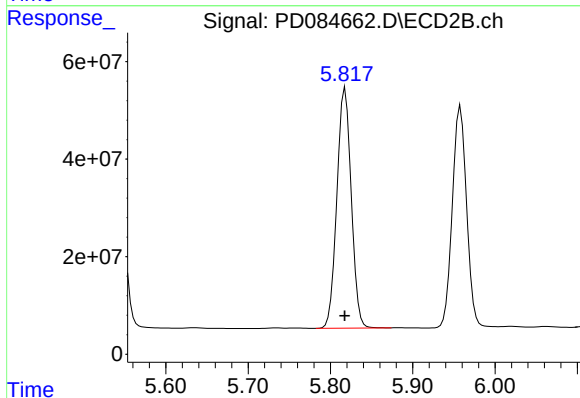


#14 Endrin

R.T.: 5.818 min
Delta R.T.: 0.000 min
Response: 596234903
Conc: 159.93 ng/ml

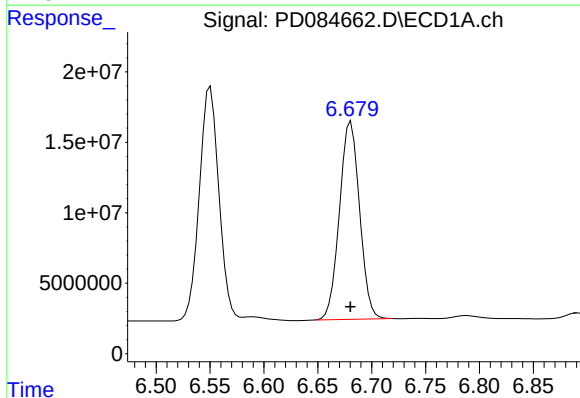


#16 4,4'-DDD

R.T.: 6.681 min
Delta R.T.: 0.000 min
Response: 182625753
Conc: 186.68 ng/ml

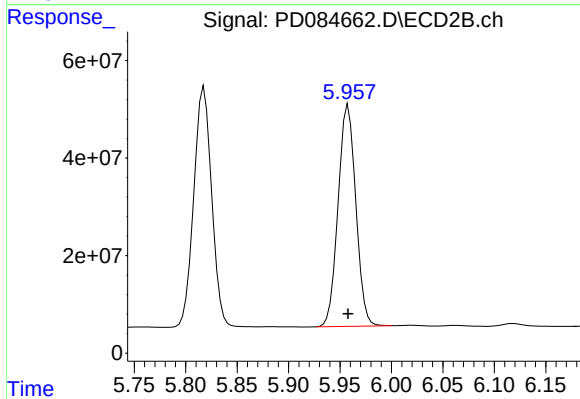


#16 4,4'-DDD

R.T.: 5.958 min
Delta R.T.: 0.000 min
Response: 544281134
Conc: 158.96 ng/ml

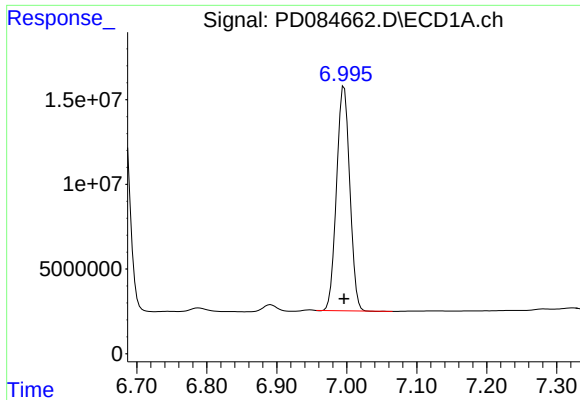


#17 4,4'-DDT

R.T.: 6.996 min
Delta R.T.: 0.000 min
Response: 174192981
Conc: 196.64 ng/ml

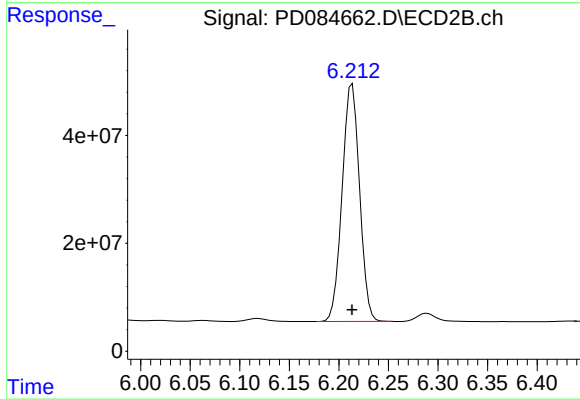


#17 4,4'-DDT

R.T.: 6.213 min
Delta R.T.: 0.000 min
Response: 538319064
Conc: 166.53 ng/ml

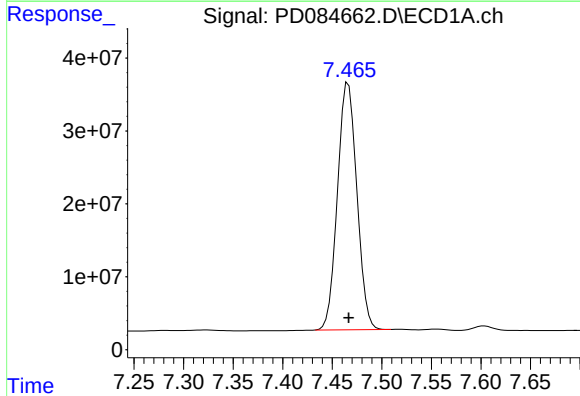


#20 Methoxychlor

R.T.: 7.466 min
Delta R.T.: 0.000 min
Response: 461780176
Conc: 879.67 ng/ml

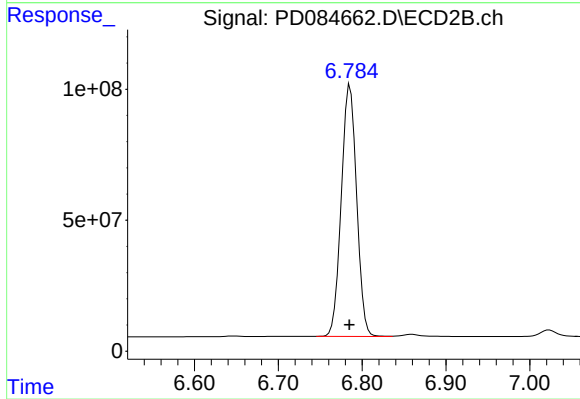

#20 Methoxychlor

R.T.: 6.786 min
Delta R.T.: 0.000 min
Response: 1223678888
Conc: 725.64 ng/ml

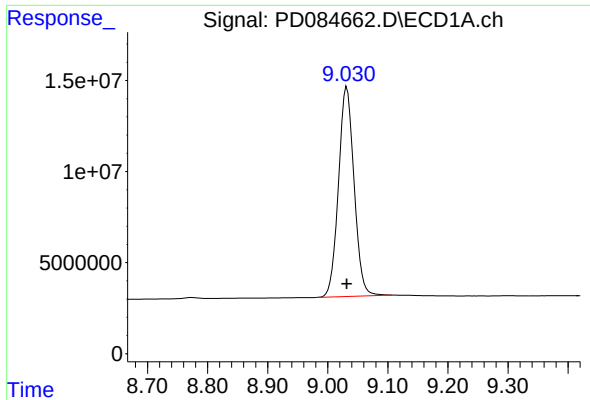


#27 Decachlorobiphenyl

R.T.: 9.032 min

Delta R.T.: 0.000 min

Response: 207250912

Conc: 158.01 ng/ml

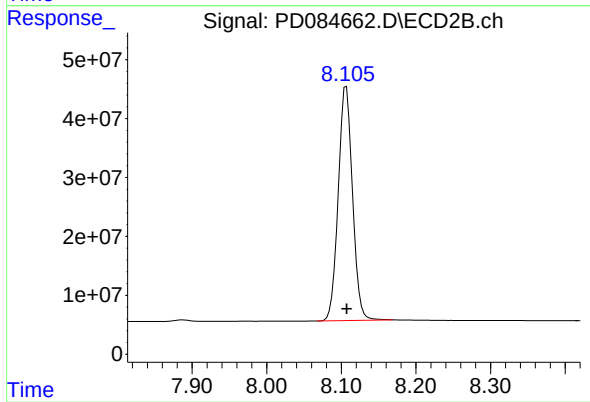

#27 Decachlorobiphenyl

R.T.: 8.107 min

Delta R.T.: 0.000 min

Response: 528585199

Conc: 150.61 ng/ml