

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082524\
 Data File : PD084663.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2024 02:47
 Operator : AR\AJ
 Sample : INDB501
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 02:24:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:21:37 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.906	83751818	283.6E6	81.061	77.305
27)	SA Decachlor...	9.032	8.107	209.9E6	531.7E6	159.989	150.022
Target Compounds							
5)	MB Aldrin	5.250	4.394	144.3E6	354.7E6	91.356	78.779
6)	B beta-BHC	4.495	4.045	59741574	165.6E6	81.956	74.891
7)	B delta-BHC	4.742	4.283	155.0E6	408.9E6	96.455	81.690
8)	B Heptachlo...	5.670	4.898	128.9E6	331.1E6	87.909	77.274
10)	B trans-Chl...	5.924	5.152	124.4E6	324.9E6	89.020	78.167
11)	B cis-Chlor...	6.004	5.217	128.6E6	327.8E6	87.504	77.235
12)	B 4,4'-DDE	6.173	5.402	245.9E6	635.9E6	200.255	160.339
15)	B Endosulfa...	6.761	6.110	223.3E6	579.9E6	175.817	154.248
18)	B Endrin al...	6.890	6.289	153.5E6	433.5E6	170.907	152.409
19)	B Endosulfa...	7.123	6.513	204.2E6	551.8E6	178.534	153.164
21)	B Endrin ke...	7.603	7.023	219.8E6	658.9E6	180.212	150.523


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082524\
Data File : PD084663.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2024 02:47
Operator : AR\AJ
Sample : INDB501
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 02:24:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:21:37 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

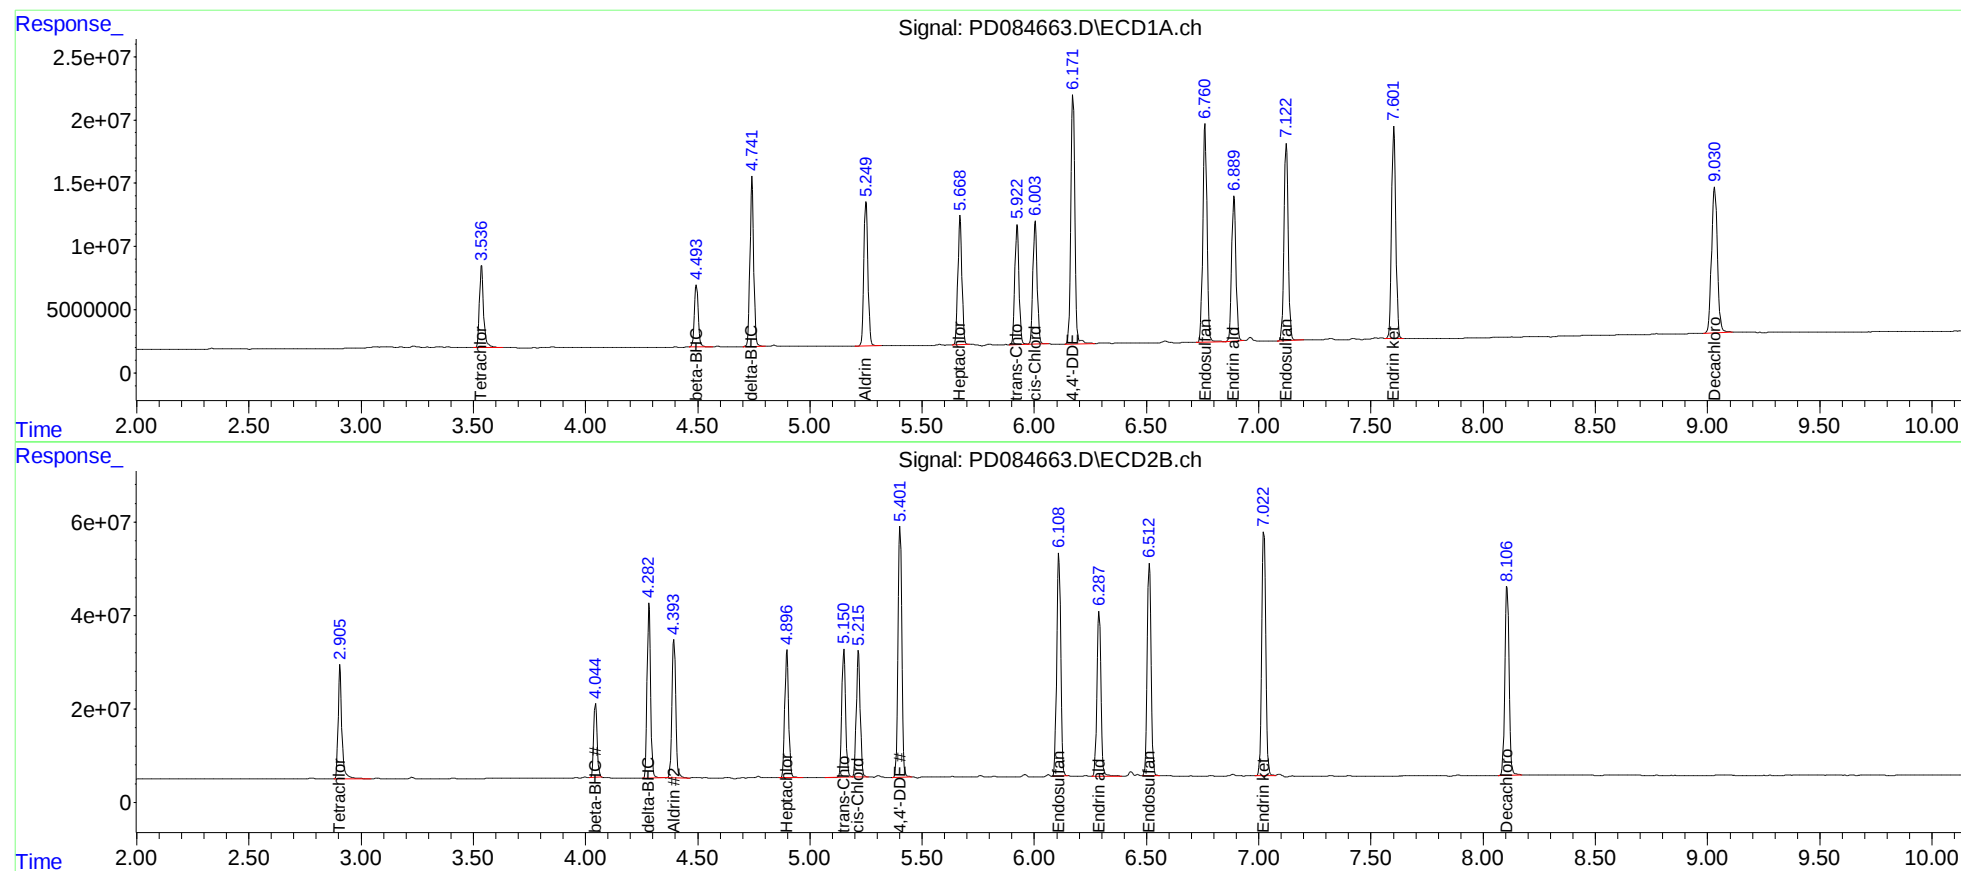

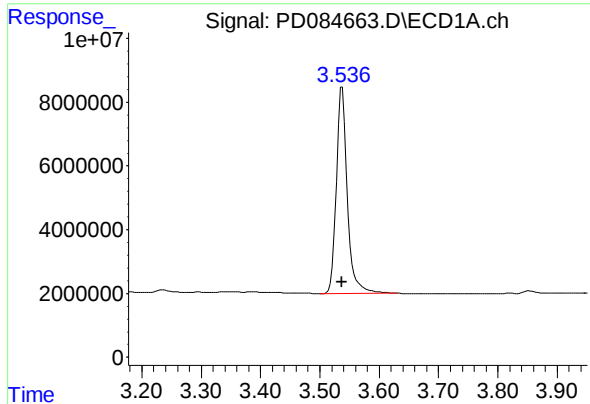


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 83751818
Conc: 81.06 ng/ml

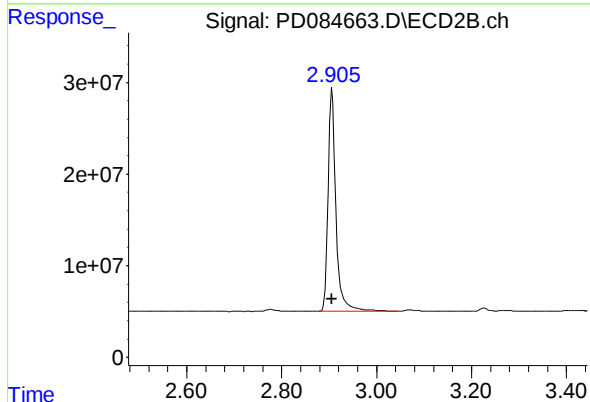


#1 Tetrachloro-m-xylene

R.T.: 2.906 min
Delta R.T.: 0.000 min
Response: 283606558
Conc: 77.30 ng/ml

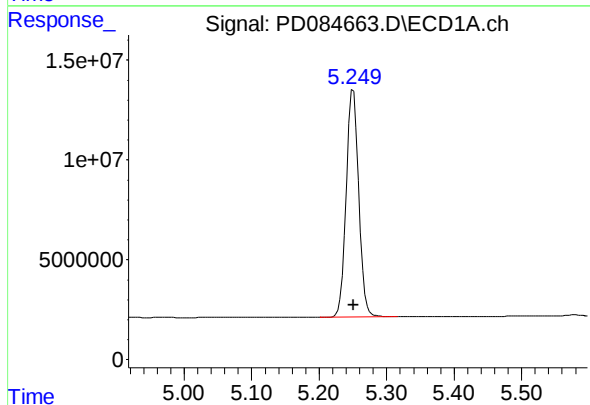


#5 Aldrin

R.T.: 5.250 min
Delta R.T.: 0.000 min
Response: 144294889
Conc: 91.36 ng/ml

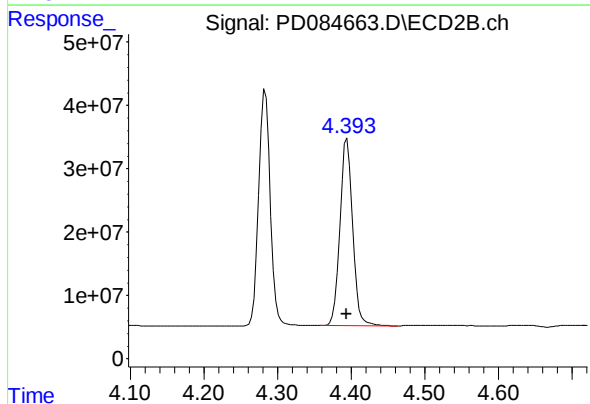


#5 Aldrin

R.T.: 4.394 min
Delta R.T.: 0.000 min
Response: 354699277
Conc: 78.78 ng/ml

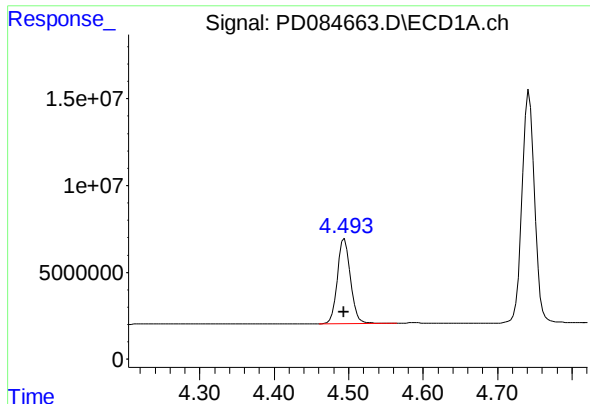


#6 beta-BHC

R.T.: 4.495 min
Delta R.T.: 0.000 min
Response: 59741574
Conc: 81.96 ng/ml

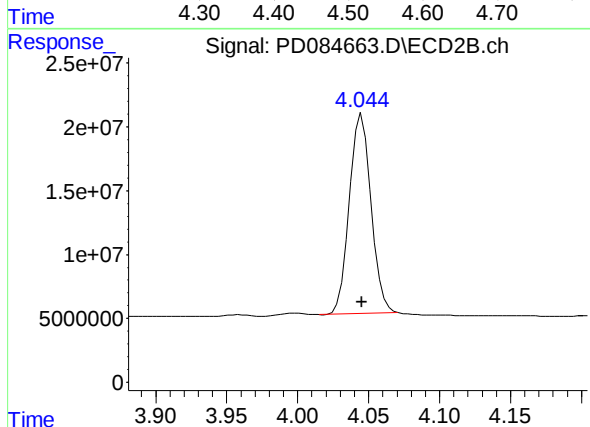


#6 beta-BHC

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 165592522
Conc: 74.89 ng/ml

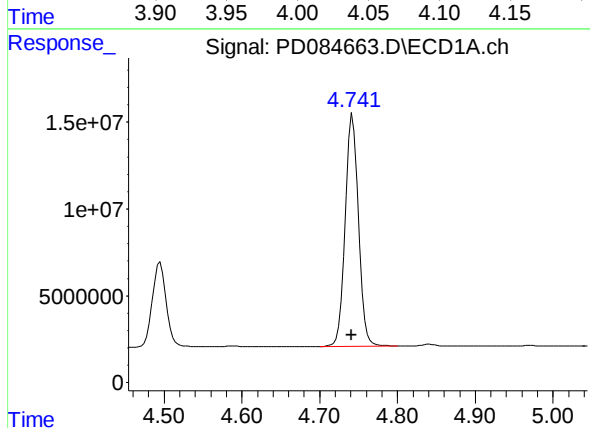


#7 delta-BHC

R.T.: 4.742 min
Delta R.T.: 0.001 min
Response: 154972825
Conc: 96.46 ng/ml

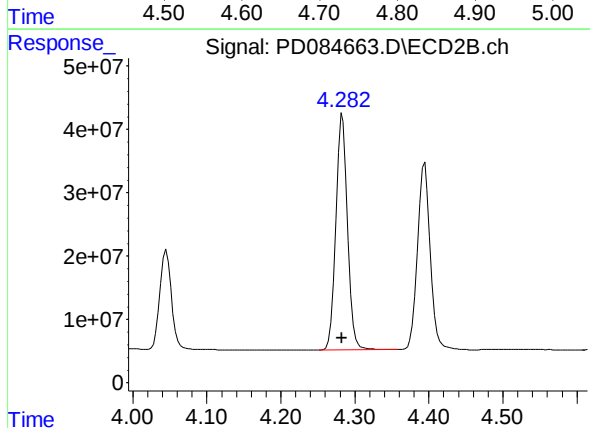


#7 delta-BHC

R.T.: 4.283 min
Delta R.T.: 0.000 min
Response: 408916666
Conc: 81.69 ng/ml

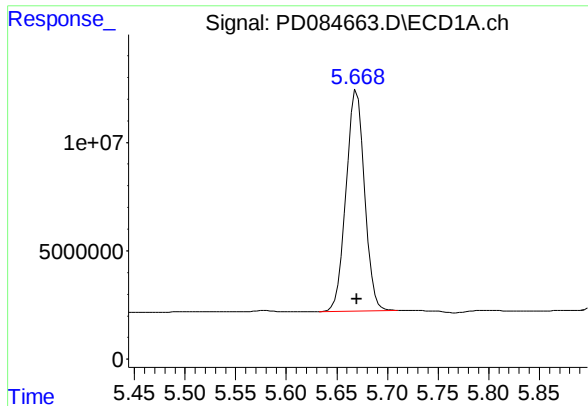


#8 Heptachlor epoxide

R.T.: 5.670 min
Delta R.T.: 0.000 min
Response: 128919773
Conc: 87.91 ng/ml

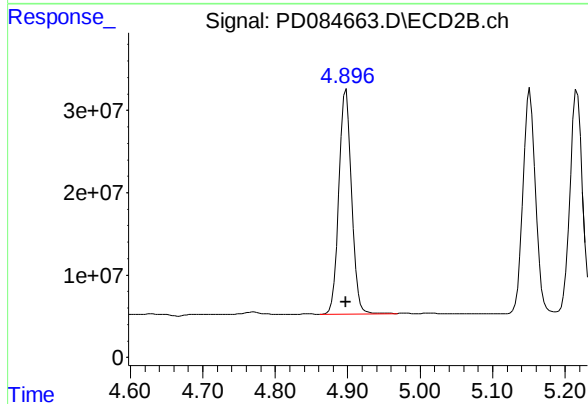


#8 Heptachlor epoxide

R.T.: 4.898 min
Delta R.T.: 0.000 min
Response: 331110787
Conc: 77.27 ng/ml

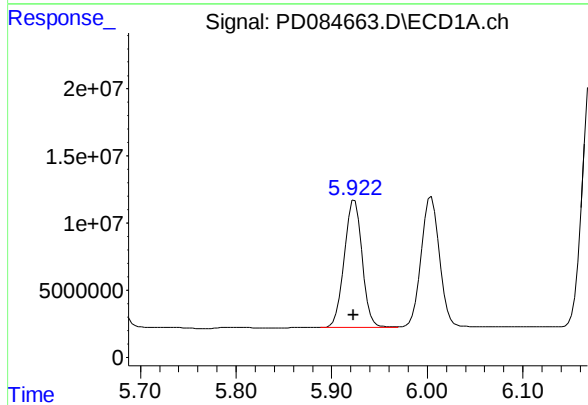


#10 trans-Chlordane

R.T.: 5.924 min
Delta R.T.: 0.000 min
Response: 124354805
Conc: 89.02 ng/ml

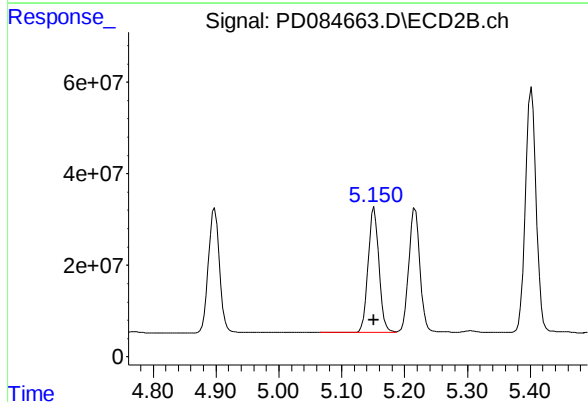


#10 trans-Chlordane

R.T.: 5.152 min
Delta R.T.: 0.000 min
Response: 324856842
Conc: 78.17 ng/ml

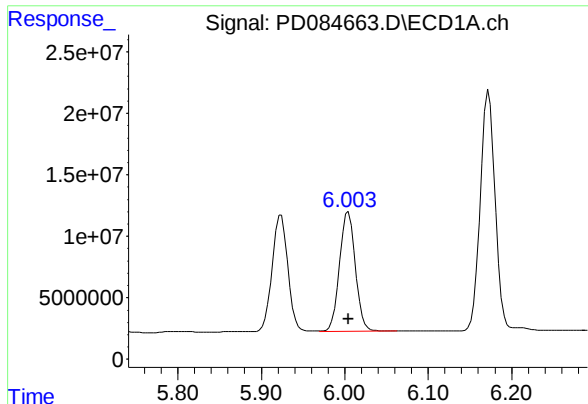


#11 cis-Chlordane

R.T.: 6.004 min
Delta R.T.: 0.000 min
Response: 128552464
Conc: 87.50 ng/ml

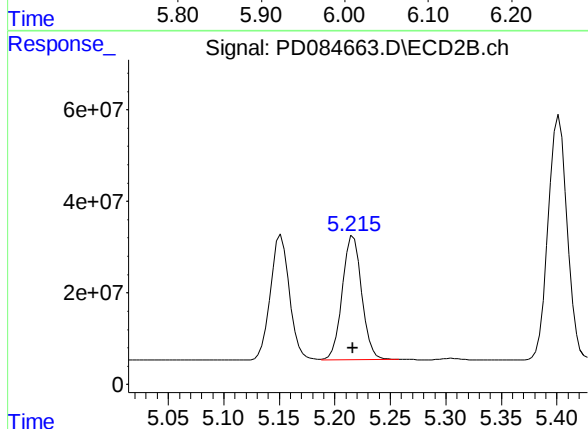


#11 cis-Chlordane

R.T.: 5.217 min
Delta R.T.: 0.000 min
Response: 327820277
Conc: 77.24 ng/ml

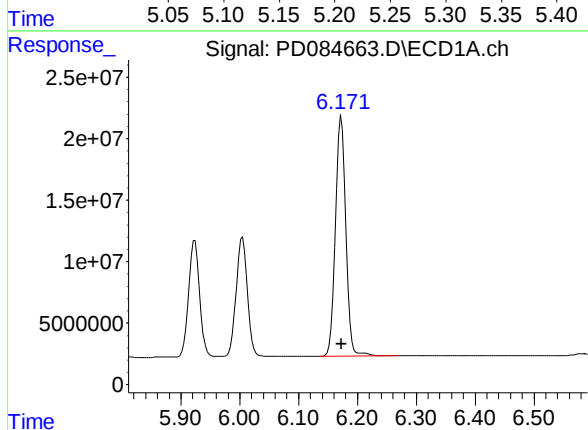


#12 4,4'-DDE

R.T.: 6.173 min
Delta R.T.: 0.000 min
Response: 245903222
Conc: 200.25 ng/ml

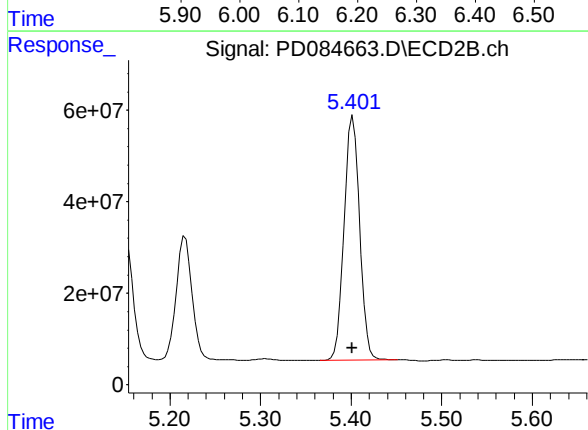


#12 4,4'-DDE

R.T.: 5.402 min
Delta R.T.: 0.000 min
Response: 635857886
Conc: 160.34 ng/ml

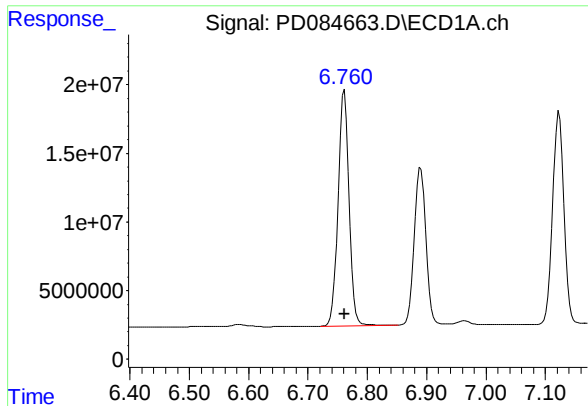


#15 Endosulfan II

R.T.: 6.761 min
Delta R.T.: 0.000 min
Response: 223288500
Conc: 175.82 ng/ml

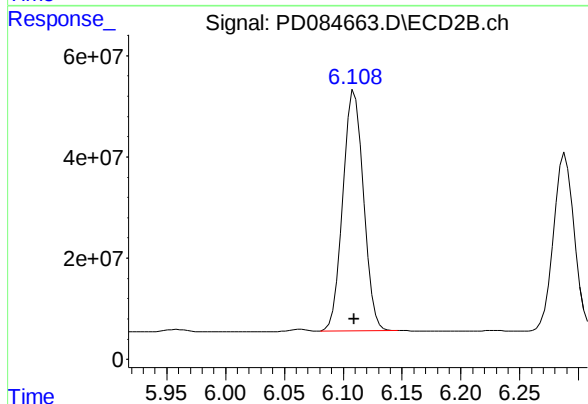


#15 Endosulfan II

R.T.: 6.110 min
Delta R.T.: 0.000 min
Response: 579936880
Conc: 154.25 ng/ml

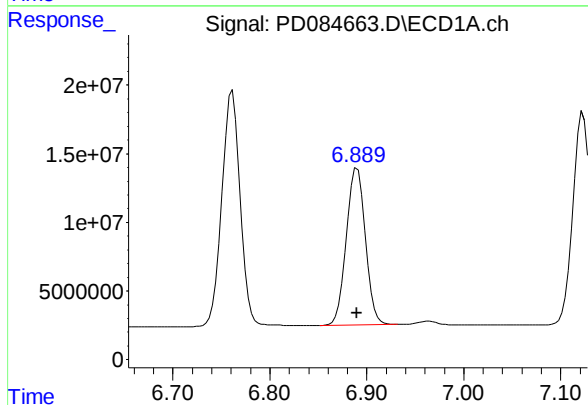


#18 Endrin aldehyde

R.T.: 6.890 min
Delta R.T.: 0.000 min
Response: 153527900
Conc: 170.91 ng/ml

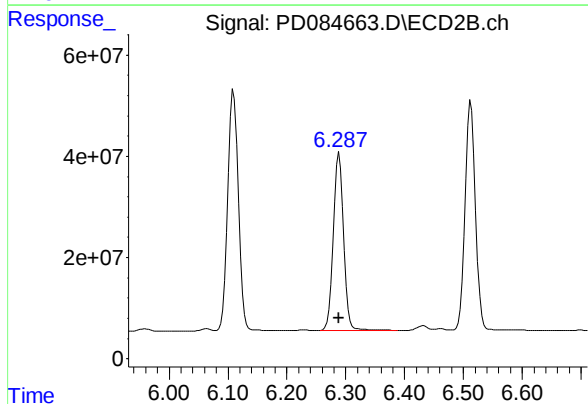


#18 Endrin aldehyde

R.T.: 6.289 min
Delta R.T.: 0.000 min
Response: 433548161
Conc: 152.41 ng/ml

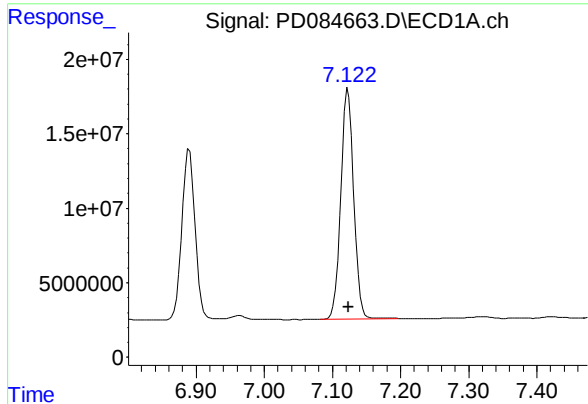


#19 Endosulfan Sulfate

R.T.: 7.123 min
Delta R.T.: 0.000 min
Response: 204162277
Conc: 178.53 ng/ml

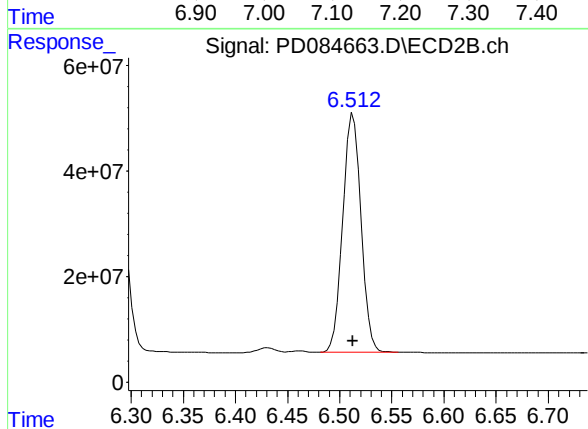


#19 Endosulfan Sulfate

R.T.: 6.513 min
Delta R.T.: 0.000 min
Response: 551761778
Conc: 153.16 ng/ml

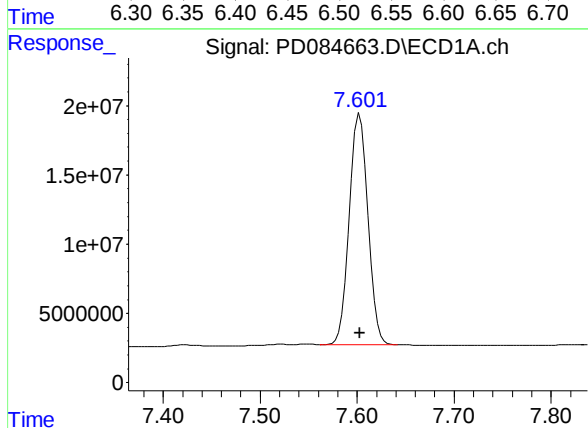


#21 Endrin ketone

R.T.: 7.603 min
Delta R.T.: 0.000 min
Response: 219763365
Conc: 180.21 ng/ml

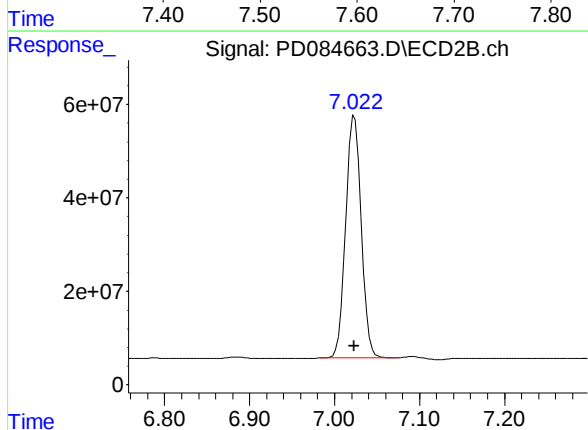


#21 Endrin ketone

R.T.: 7.023 min
Delta R.T.: 0.000 min
Response: 658858960
Conc: 150.52 ng/ml

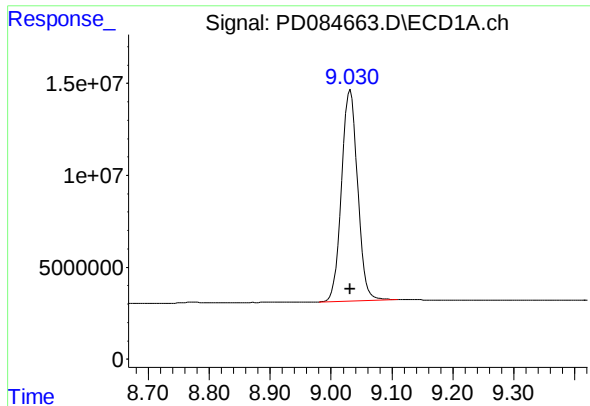

#27 Decachlorobiphenyl

R.T.: 9.032 min
Delta R.T.: 0.000 min
Response: 209929242
Conc: 159.99 ng/ml

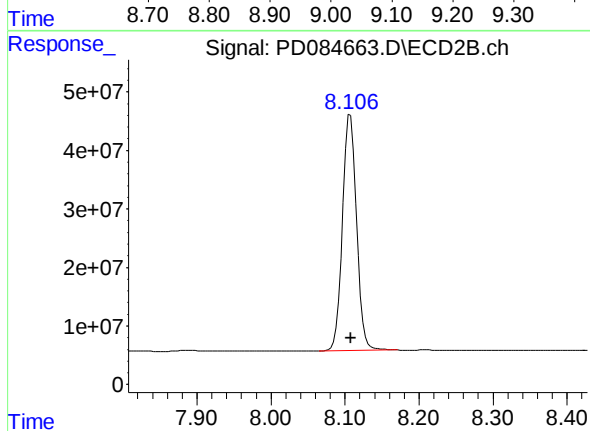

#27 Decachlorobiphenyl

R.T.: 8.107 min
Delta R.T.: 0.000 min
Response: 531696546
Conc: 150.02 ng/ml