

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082524\
 Data File : PD084647.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2024 23:00
 Operator : AR\AJ
 Sample : RESC043
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC046

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 04:55:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.906	20319826	73772332	20.091	20.847
2)	SA Decachlor...	9.033	8.107	52997395	141.7E6	40.579	40.750
Target Compounds							
2)	A alpha-BHC	3.983	3.417	16513754	53951368	9.713	10.641
3)	MA gamma-BHC...	4.312	3.752	16008854	52303538	9.895	10.794
4)	MA Heptachlor	4.909	4.107	15742361	45486719	10.232	10.685
5)	MB Aldrin	5.250	4.394	15100630	49485571	9.442	11.142
6)	B beta-BHC	4.495	4.045	6984079	21966672	9.615	10.132
7)	B delta-BHC	4.742	4.283	14932983	48826066	9.105	9.836
8)	B Heptachlo...	5.669	4.898	14121171	42306465	9.468	9.989
9)	A Endosulfan I	6.052	5.274	14313986	42026247	10.404	10.963
10)	B trans-Chl...	5.924	5.152	13046200	41605428	9.250	10.115
11)	B cis-Chlor...	6.005	5.217	13657385	42403017	9.237	10.106
12)	B 4,4'-DDE	6.173	5.402	23327865	77481964	18.700	19.753
13)	MA Dieldrin	6.324	5.541	29476900	92985221	19.983	21.644
14)	MA Endrin	6.551	5.818	22327339	82191244	19.788	22.200
15)	B Endosulfa...	6.761	6.110	25372454	73431427	19.221	19.805
16)	A 4,4'-DDD	6.681	5.959	19941213	73965504	20.197	21.796
17)	MA 4,4'-DDT	6.997	6.214	17580847	69441044	19.641	21.708
18)	B Endrin al...	6.891	6.289	17212085	57254853	19.059	20.053
19)	B Endosulfa...	7.124	6.513	21586609	71590330	18.738	20.045
20)	A Methoxychlor	7.468	6.786	54323027	189.1E6	104.284	114.288
21)	B Endrin ke...	7.604	7.024	23635238	94875137	19.331	21.547

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082524\
Data File : PD084647.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2024 23:00
Operator : AR\AJ
Sample : RESC043
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 04:55:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

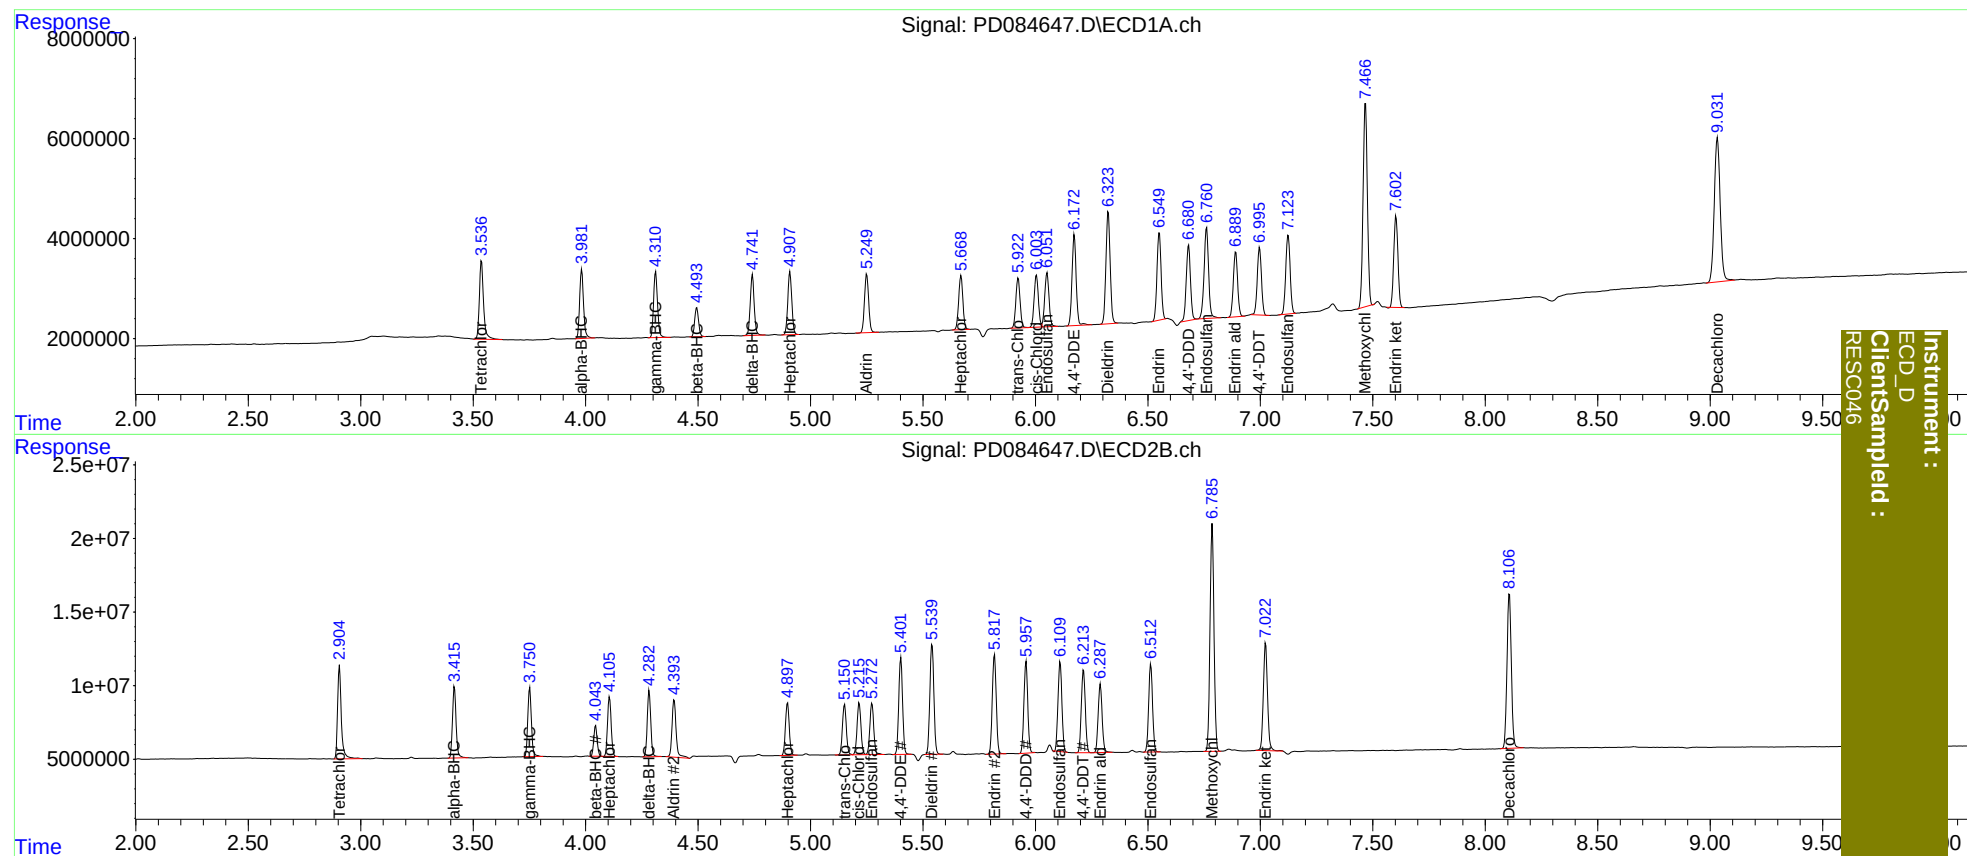

Instrument :
ECD_D
ClientSampled :
RESC046

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082524\
Data File : PD084647.D
Acq On : 22 Aug 2024 23:00
Operator : AR\AJ
Sample : RESC043
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC046

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Title : GC Extractables
Last Update : Tue Aug 27 02:47:48 2024
Integrator: ChemStation

RT#1	RT#2	Resolution
3.537	3.983	100.00%
3.983	4.312	100.00%
4.312	4.495	100.00%
4.495	4.742	100.00%
4.742	4.909	100.00%
4.909	5.250	100.00%
5.250	5.669	100.00%
5.669	5.924	100.00%
5.924	6.005	99.72%
6.005	6.052	94.22%
6.052	6.173	100.00%
6.173	6.324	100.00%
6.324	6.551	100.00%
6.551	6.681	100.00%
6.681	6.761	100.00%
6.761	6.891	100.00%
6.891	6.997	100.00%
6.997	7.124	100.00%
7.124	7.468	100.00%
7.468	7.604	100.00%
7.604	9.033	100.00%

Signal #2


2.906	3.417	100.00%
3.417	3.752	100.00%
3.752	4.045	100.00%
4.045	4.107	100.00%
4.107	4.283	100.00%
4.283	4.394	100.00%
4.394	4.898	100.00%
4.898	5.152	100.00%
5.152	5.217	100.00%
5.217	5.274	100.00%
5.274	5.402	100.00%
5.402	5.541	100.00%
5.541	5.818	100.00%
5.818	5.959	100.00%
5.959	6.110	100.00%
6.110	6.214	100.00%
6.214	6.289	100.00%
6.289	6.513	100.00%
6.513	6.786	100.00%
6.786	7.024	100.00%
7.024	8.107	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082524\
Data File : PD084647.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2024 23:00
Operator : AR\AJ
Sample : RESC043
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC046

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 04:55:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

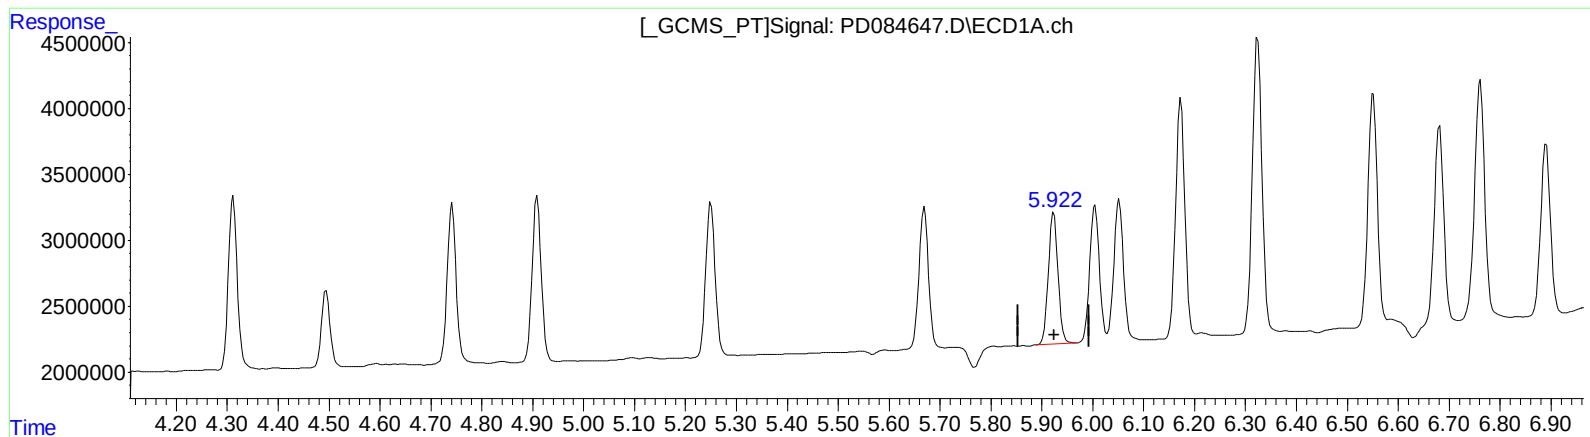

(10) trans-Chlordane (B)

5.924min 9.250 ng/ml

response 13046200

(10) trans-Chlordane #2 (B)

5.152min 10.115 ng/ml



response 41605428

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082524\
Data File : PD084647.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2024 23:00
Operator : AR\AJ
Sample : RESC043
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC046

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 04:55:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

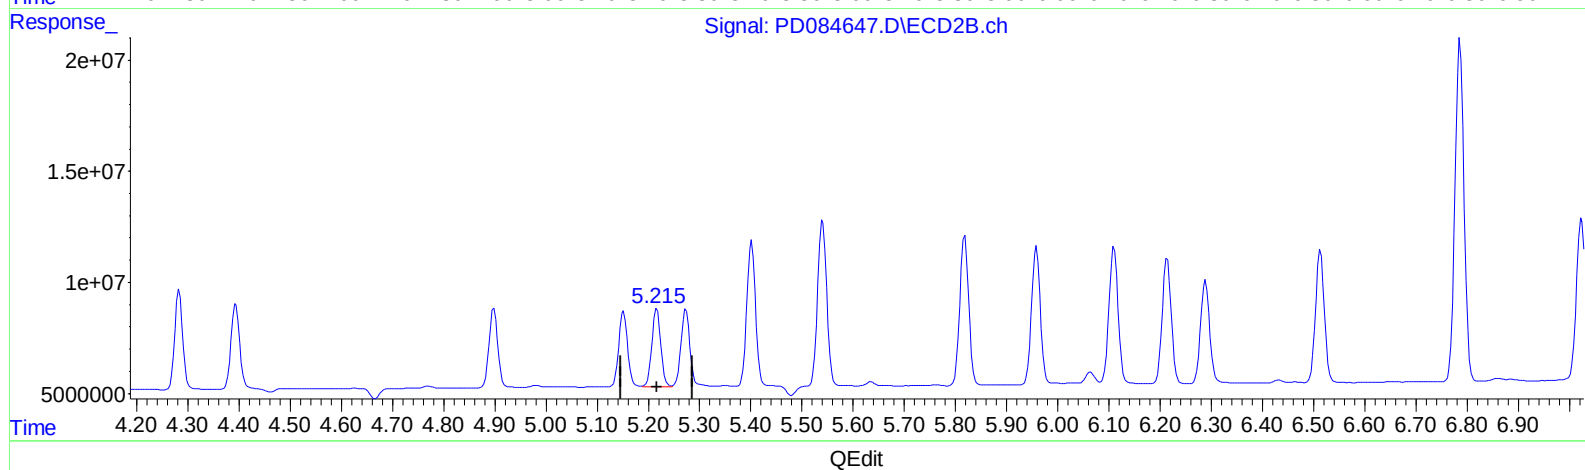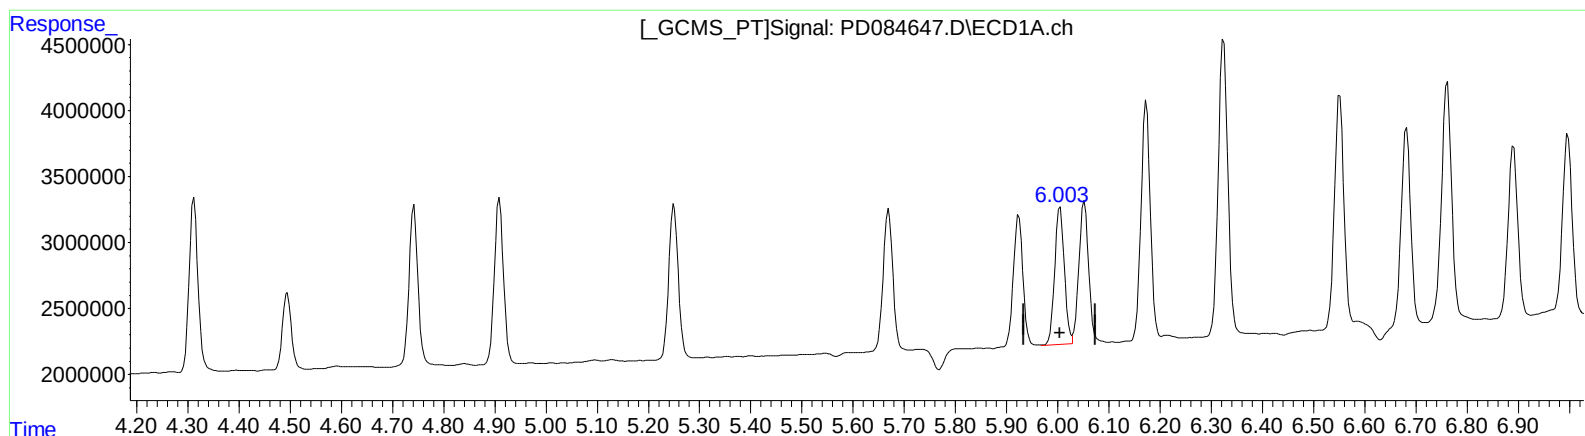

(11) cis-Chlordane (B)
6.005min 9.237 ng/ml
response 13657385

(11) cis-Chlordane #2 (B)
5.217min 10.106 ng/ml
response 42403017