

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082620\
 Data File : PD059065.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Aug 2020 09:48
 Operator : DD\AJ
 Sample : PIBLK47
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK47

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 04:41:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 11:29:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.207	3.865	20228454	32220316	20.917	22.248
27) SA Decachlor...	7.842	8.861	33376803	43033850	31.688	31.379
Target Compounds						
8) B Heptachlo...	0.000	5.709	0	3205676	N.D.	1.925


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082620\
Data File : PD059065.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2020 09:48
Operator : DD\AJ
Sample : PIBLK47
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK47

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 04:41:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 11:29:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

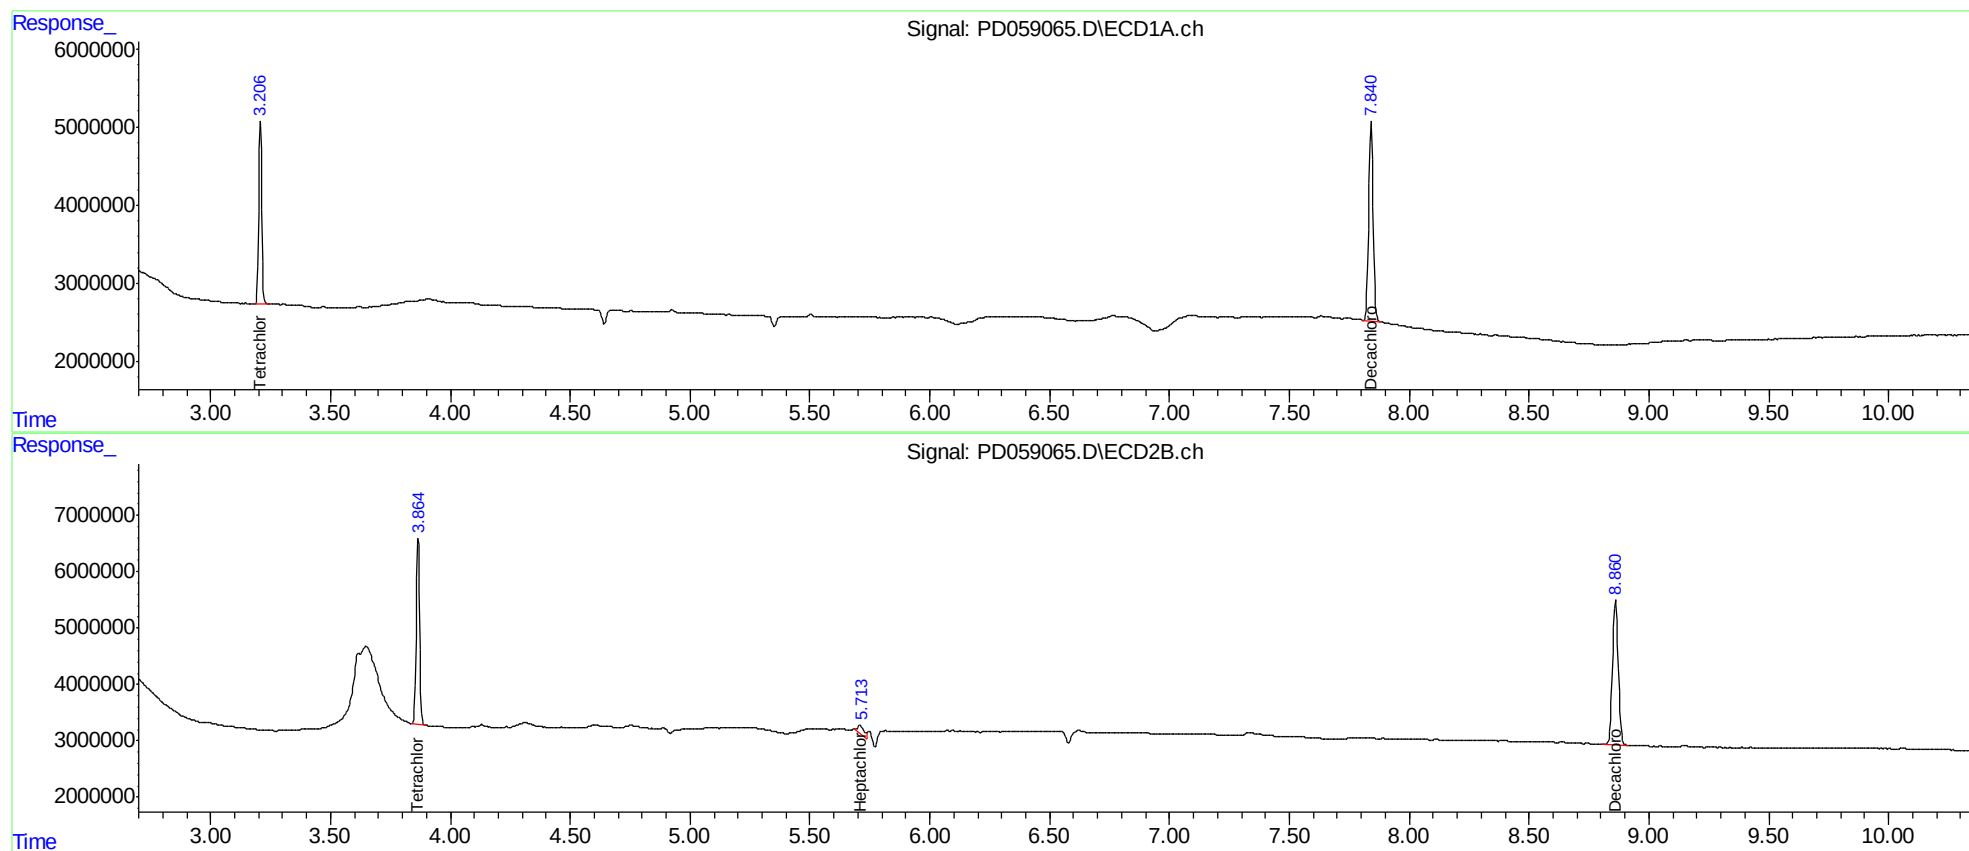


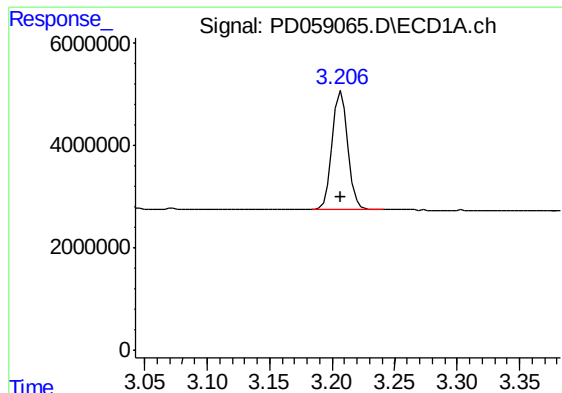

#1 Tetrachloro-m-xylene


R.T.: 3.207 min
Delta R.T.: 0.000 min
Response: 20228454
Conc: 20.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK47

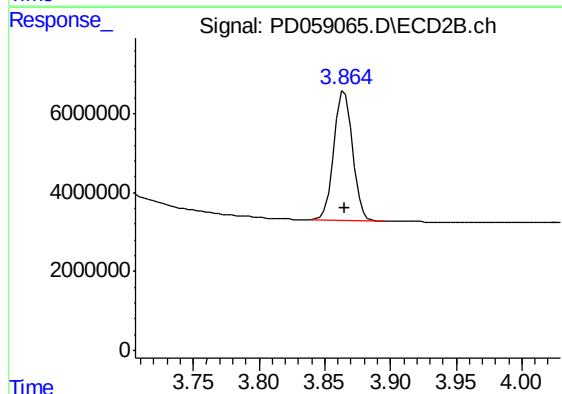


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 32220316
Conc: 22.25 ng/ml

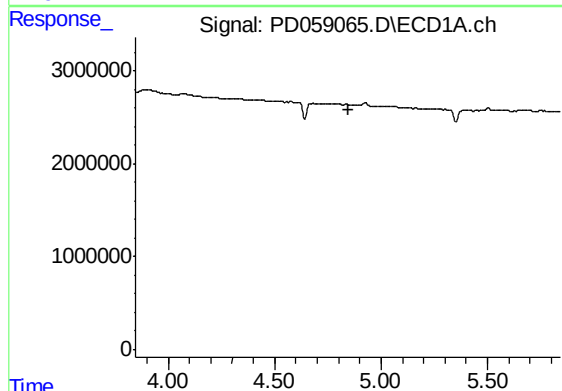


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.846 min
Response: 0
Conc: N.D.

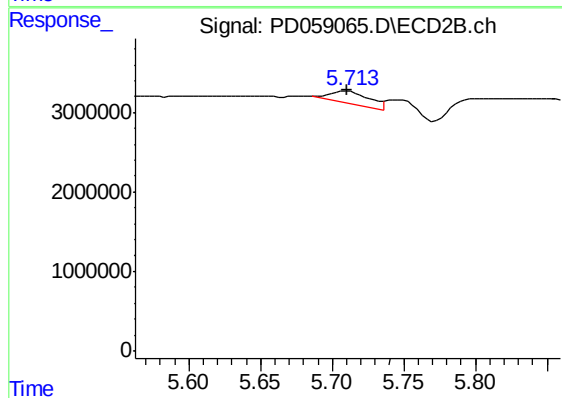

#8 Heptachlor epoxide


R.T.: 5.709 min
Delta R.T.: -0.002 min
Response: 3205676
Conc: 1.93 ng/ml

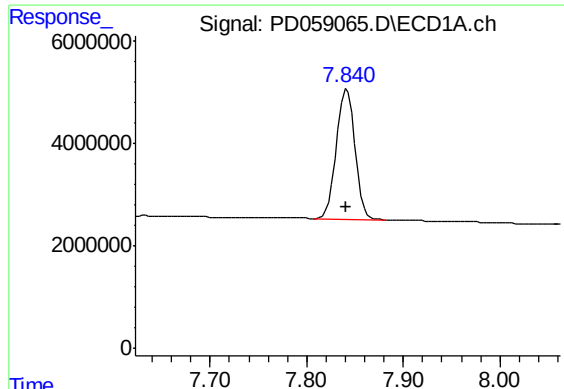

#27 Decachlorobiphenyl

R.T.: 7.842 min
Delta R.T.: 0.001 min
Response: 33376803
Conc: 31.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK47

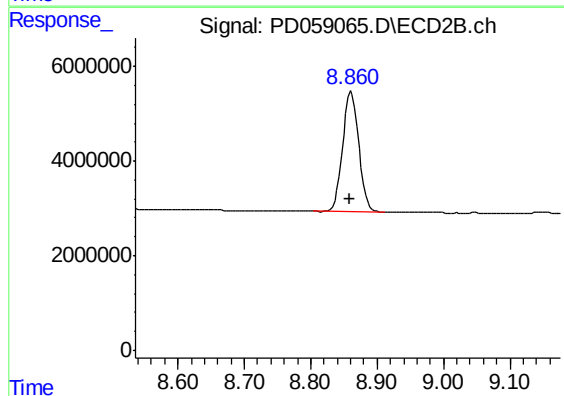

#27 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.003 min
Response: 43033850
Conc: 31.38 ng/ml