

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082622\
 Data File : PD071689.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Aug 2022 22:35
 Operator : AR\AJ
 Sample : N4320-07MS
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AX9MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/29/2022
 Supervised By :Ankita Jodhani 08/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 07:26:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 27 07:11:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.806	3.563	43084320	535.7E6	16.521	16.347
27)	SA Decachlor...	7.996	9.088	87063435	319.3E6	33.177	33.399
Target Compounds							
2)	A alpha-BHC	3.314	4.029	219.0E6	2196.6E6	56.783	49.785
3)	MA gamma-BHC...	3.648	4.365	205.7E6	1803.7E6	55.721	48.498
4)	MA Heptachlor	3.992	4.941	196.7E6	1216.6E6	51.684m	45.056m
5)	MB Aldrin	4.277	5.284	192.7E6	999.5E6	54.139	46.267
6)	B beta-BHC	3.944	4.571	82398352	687.1E6	51.872m	48.007
7)	B delta-BHC	4.179	4.819	205.7E6	1334.5E6	58.869	50.774
8)	B Heptachlo...	4.784	5.716	187.6E6	855.0E6	57.563	50.559
9)	A Endosulfan I	5.157	6.102	171.9E6	768.1E6	54.542	48.905m
10)	B trans-Chl...	5.036	5.970	186.5E6	814.7E6	55.085	48.125
11)	B cis-Chlor...	5.101	6.046	183.7E6	797.7E6	55.070	48.945m
12)	B 4,4'-DDE	5.292	6.221	333.8E6	1417.9E6	108.838	97.172
13)	MA Dieldrin	5.424	6.380	394.0E6	1637.2E6	113.780	102.297
14)	MA Endrin	5.701	6.614	342.5E6	1347.2E6	114.354	102.391
15)	B Endosulfa...	5.996	6.839	318.7E6	1311.5E6	119.911	108.799
16)	A 4,4'-DDD	5.850	6.745	296.9E6	1234.2E6	112.816	100.862
17)	MA 4,4'-DDT	6.103	7.056	311.1E6	1276.1E6	114.277	105.759
18)	B Endrin al...	6.177	6.969	253.9E6	1039.4E6	109.745	101.878
19)	B Endosulfa...	6.401	7.202	300.6E6	1188.7E6	112.833	104.672
20)	A Methoxychlor	6.683	7.532	779.2E6	2844.9E6	542.506	518.496
21)	B Endrin ke...	6.911	7.694	365.4E6	1368.6E6	122.098	110.564

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082622\
Data File : PD071689.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2022 22:35
Operator : AR\AJ
Sample : N4320-07MS
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 07:26:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 27 07:11:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

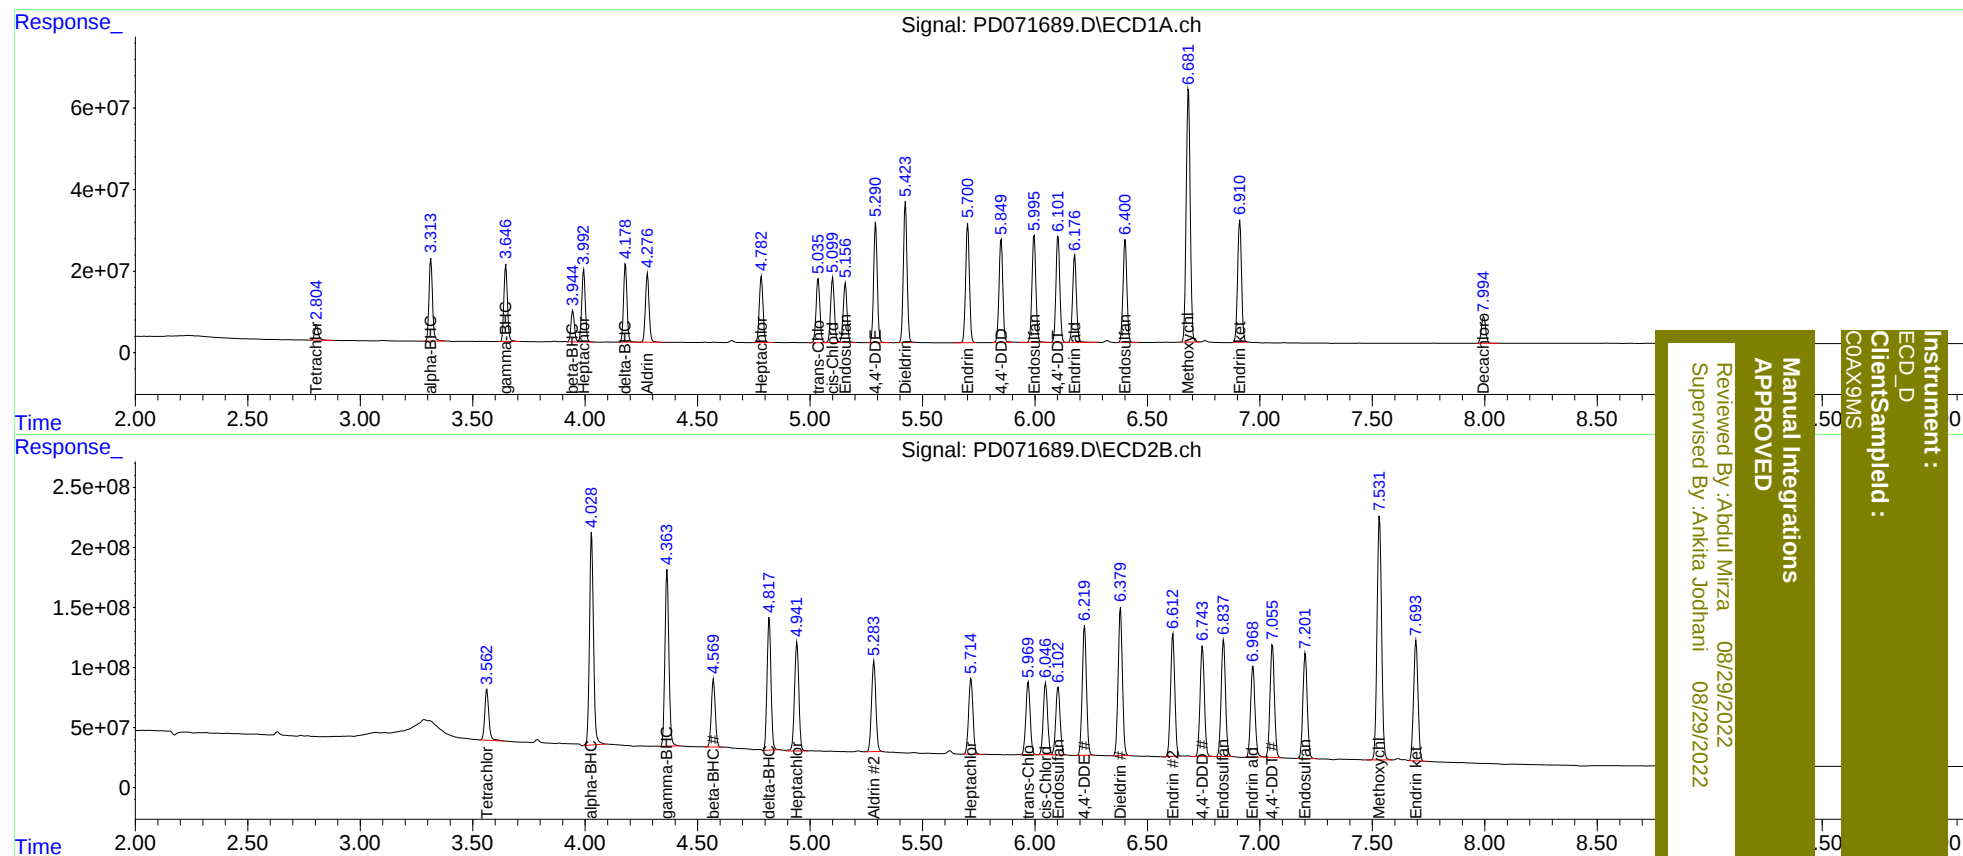

Reviewed By: Abdul Mirza 08/29/2022
Supervised By: Ankita Jodhani 08/29/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
COAX9MS