

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082622\
 Data File : PD071662.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Aug 2022 16:29
 Operator : AR\AJ
 Sample : RESC036
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC038

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 02:00:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 27 07:11:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.804	3.563	50312598	632.5E6	19.292	19.302
27)	SA Decachlor...	7.995	9.089	102.2E6	377.3E6	38.951	39.465
Target Compounds							
2)	A alpha-BHC	3.313	4.028	37681849	462.6E6	9.770	10.485
3)	MA gamma-BHC...	3.646	4.364	36567243	393.4E6	9.905	10.577
4)	MA Heptachlor	3.993	4.941	38043045	292.4E6	9.995	10.827
5)	MB Aldrin	4.277	5.284	35855333	234.8E6	10.072	10.869
6)	B beta-BHC	3.945	4.570	16303567	153.0E6	10.263	10.691
7)	B delta-BHC	4.179	4.818	34249656	267.3E6	9.801	10.170
8)	B Heptachlo...	4.783	5.716	32771678	170.2E6	10.055	10.067
9)	A Endosulfan I	5.157	6.103	31947175	168.3E6	10.137	10.717
10)	B trans-Chl...	5.036	5.970	33684992	180.0E6	9.949	10.636
11)	B cis-Chlor...	5.101	6.048	33163923	171.2E6	9.943	10.503
12)	B 4,4'-DDE	5.292	6.220	60333058	306.3E6	19.670	20.989
13)	MA Dieldrin	5.424	6.380	68646641	337.9E6	19.823	21.111
14)	MA Endrin	5.701	6.613	59679834	288.8E6	19.927	21.954
15)	B Endosulfa...	5.996	6.838	53264843	255.4E6	20.039	21.189
16)	A 4,4'-DDD	5.850	6.744	52283397	258.4E6	19.864	21.117
17)	MA 4,4'-DDT	6.104	7.056	52985000	253.2E6	19.463	20.988
18)	B Endrin al...	6.177	6.970	47462617	217.3E6	20.518	21.299
19)	B Endosulfa...	6.401	7.203	53695813	237.8E6	20.156	20.941
20)	A Methoxychlor	6.683	7.533	149.5E6	589.9E6	104.102	107.506
21)	B Endrin ke...	6.911	7.694	61871221	264.8E6	20.675	21.390

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082622\
Data File : PD071662.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2022 16:29
Operator : AR\AJ
Sample : RESC036
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 02:00:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 27 07:11:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

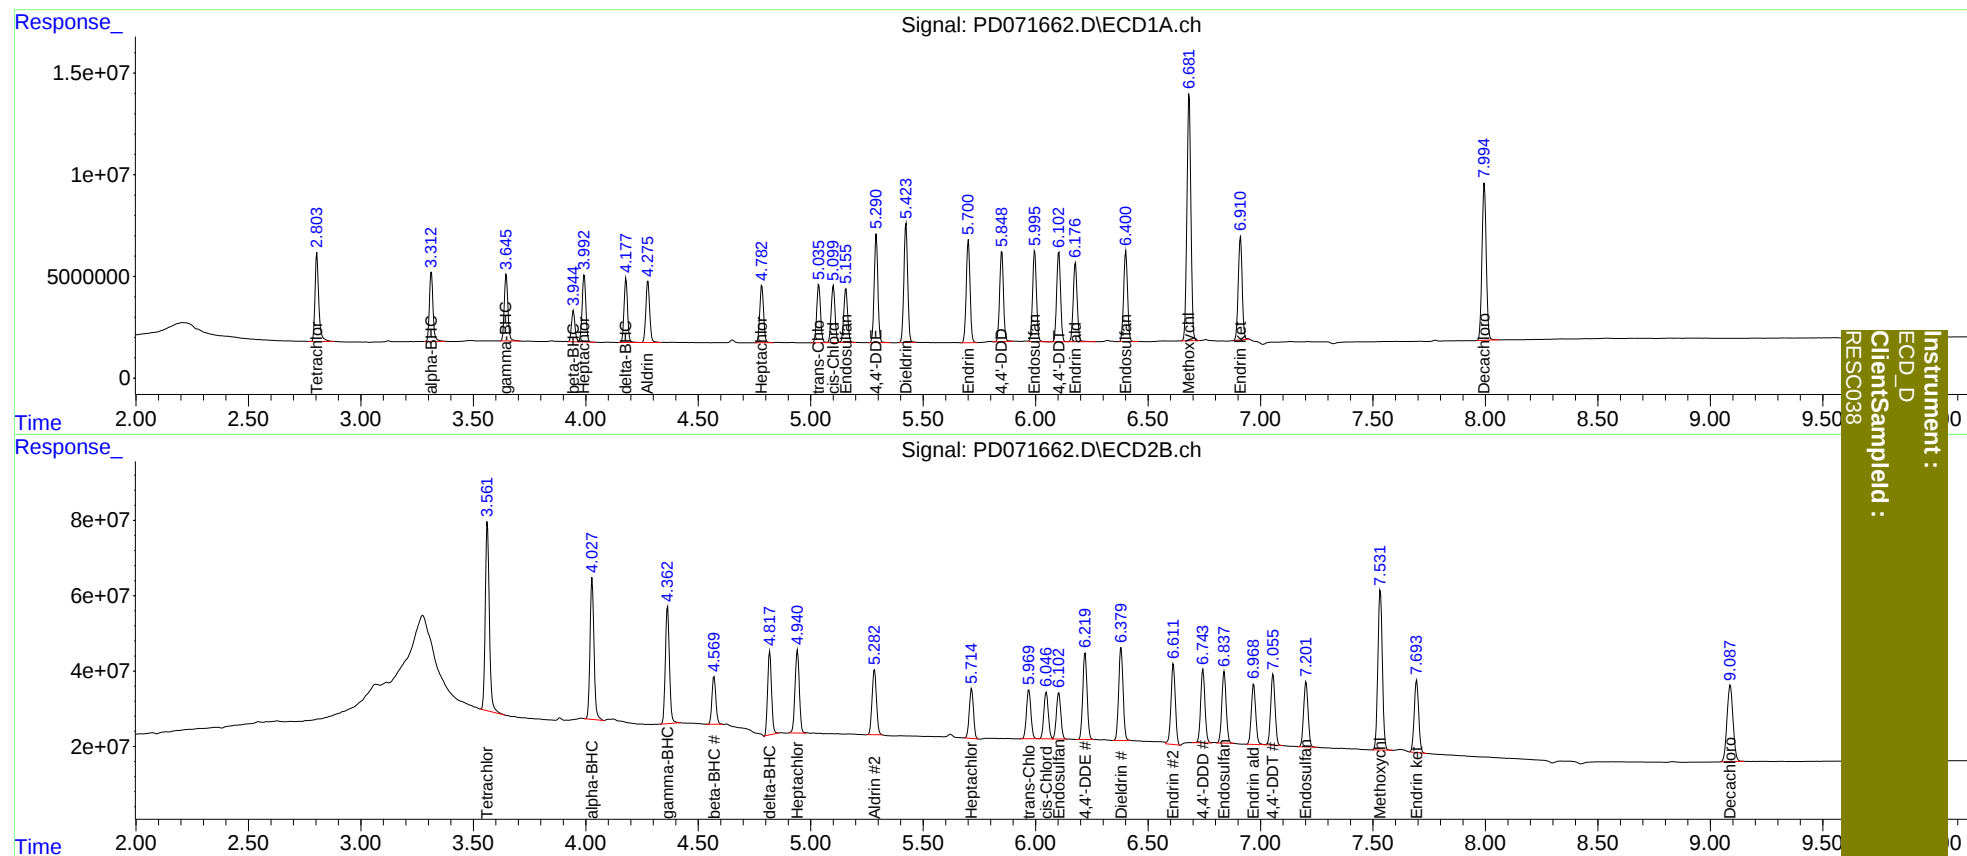

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082622\
Data File : PD071662.D
Acq On : 26 Aug 2022 16:29
Operator : AR\AJ
Sample : RESC036
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC038

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
Title : GC Extractables
Last Update : Sat Aug 27 07:11:22 2022
Integrator: ChemStation

RT#1	RT#2	Resolution
2.804	3.313	100.00%
3.313	3.646	100.00%
3.646	3.945	100.00%
3.945	3.993	99.59%
3.993	4.179	100.00%
4.179	4.277	100.00%
4.277	4.783	100.00%
4.783	5.036	100.00%
5.036	5.101	100.00%
5.101	5.157	98.66%
5.157	5.292	100.00%
5.292	5.424	100.00%
5.424	5.701	100.00%
5.701	5.850	100.00%
5.850	5.996	100.00%
5.996	6.104	99.85%
6.104	6.177	100.00%
6.177	6.401	100.00%
6.401	6.683	100.00%
6.683	6.911	100.00%
6.911	7.995	100.00%

Signal #2


3.563	4.028	100.00%
4.028	4.364	100.00%
4.364	4.570	100.00%
4.570	4.818	100.00%
4.818	4.941	100.00%
4.941	5.284	100.00%
5.284	5.716	100.00%
5.716	5.970	100.00%
5.970	6.048	100.00%
6.048	6.103	99.22%
6.103	6.220	100.00%
6.220	6.380	100.00%
6.380	6.613	100.00%
6.613	6.744	100.00%
6.744	6.838	100.00%
6.838	6.970	100.00%
6.970	7.056	100.00%
7.056	7.203	100.00%
7.203	7.533	100.00%
7.533	7.694	100.00%
7.694	9.089	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082622\
Data File : PD071662.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2022 16:29
Operator : AR\AJ
Sample : RESC036
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC038

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 02:00:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 27 07:11:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

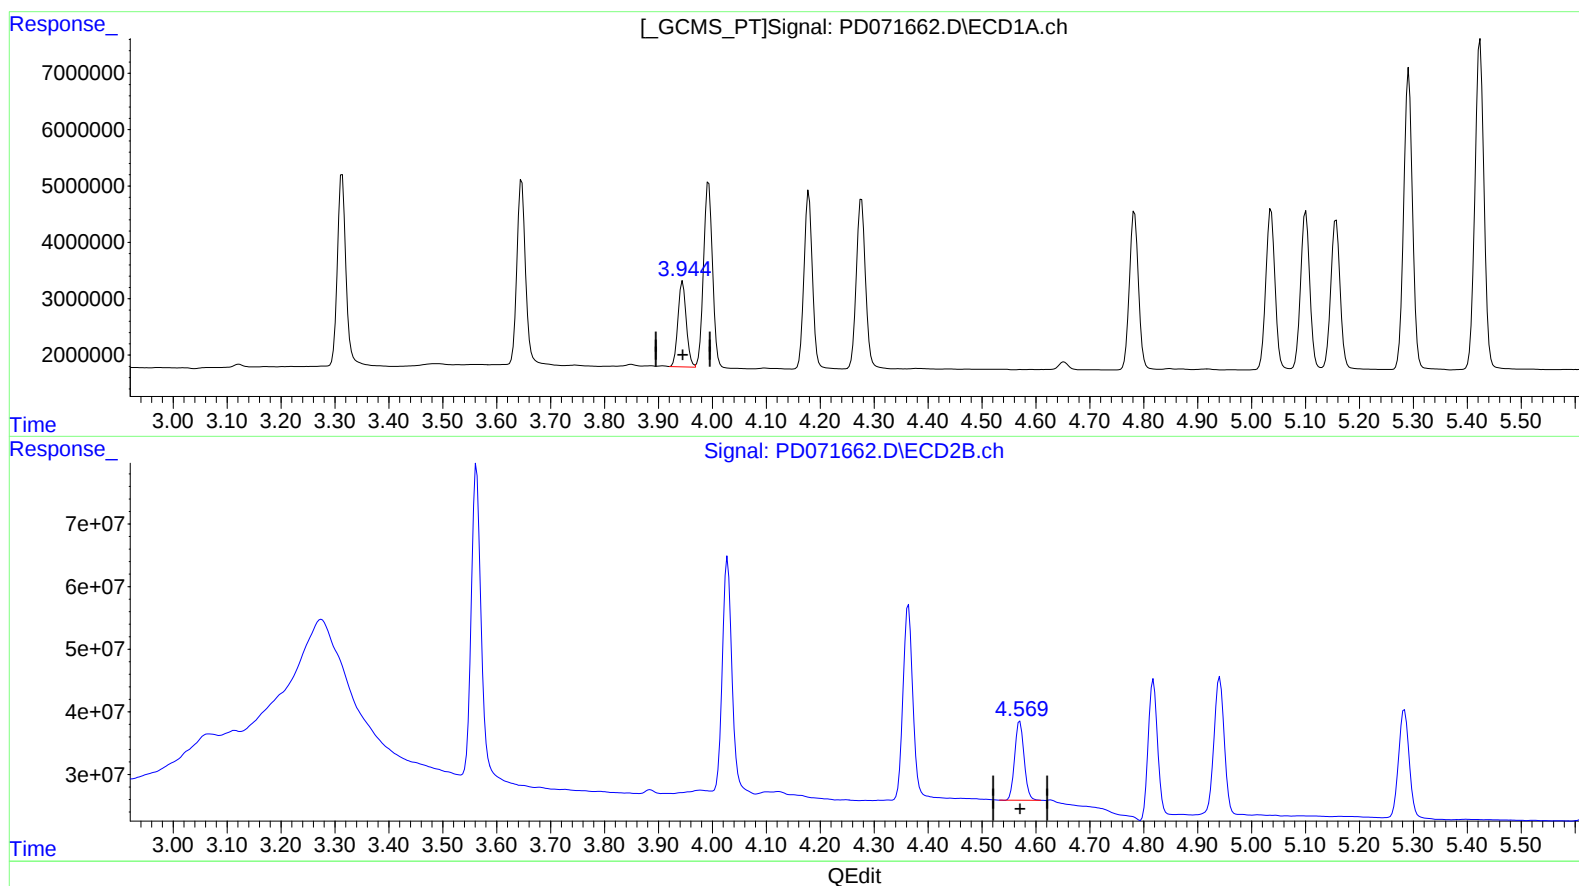

(6) beta-BHC (B)

3.945min 10.263 ng/ml

response 16303567

(6) beta-BHC #2 (B)

4.570min 10.691 ng/ml


response 153018016

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082622\
Data File : PD071662.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2022 16:29
Operator : AR\AJ
Sample : RESC036
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC038

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 02:00:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 27 07:11:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

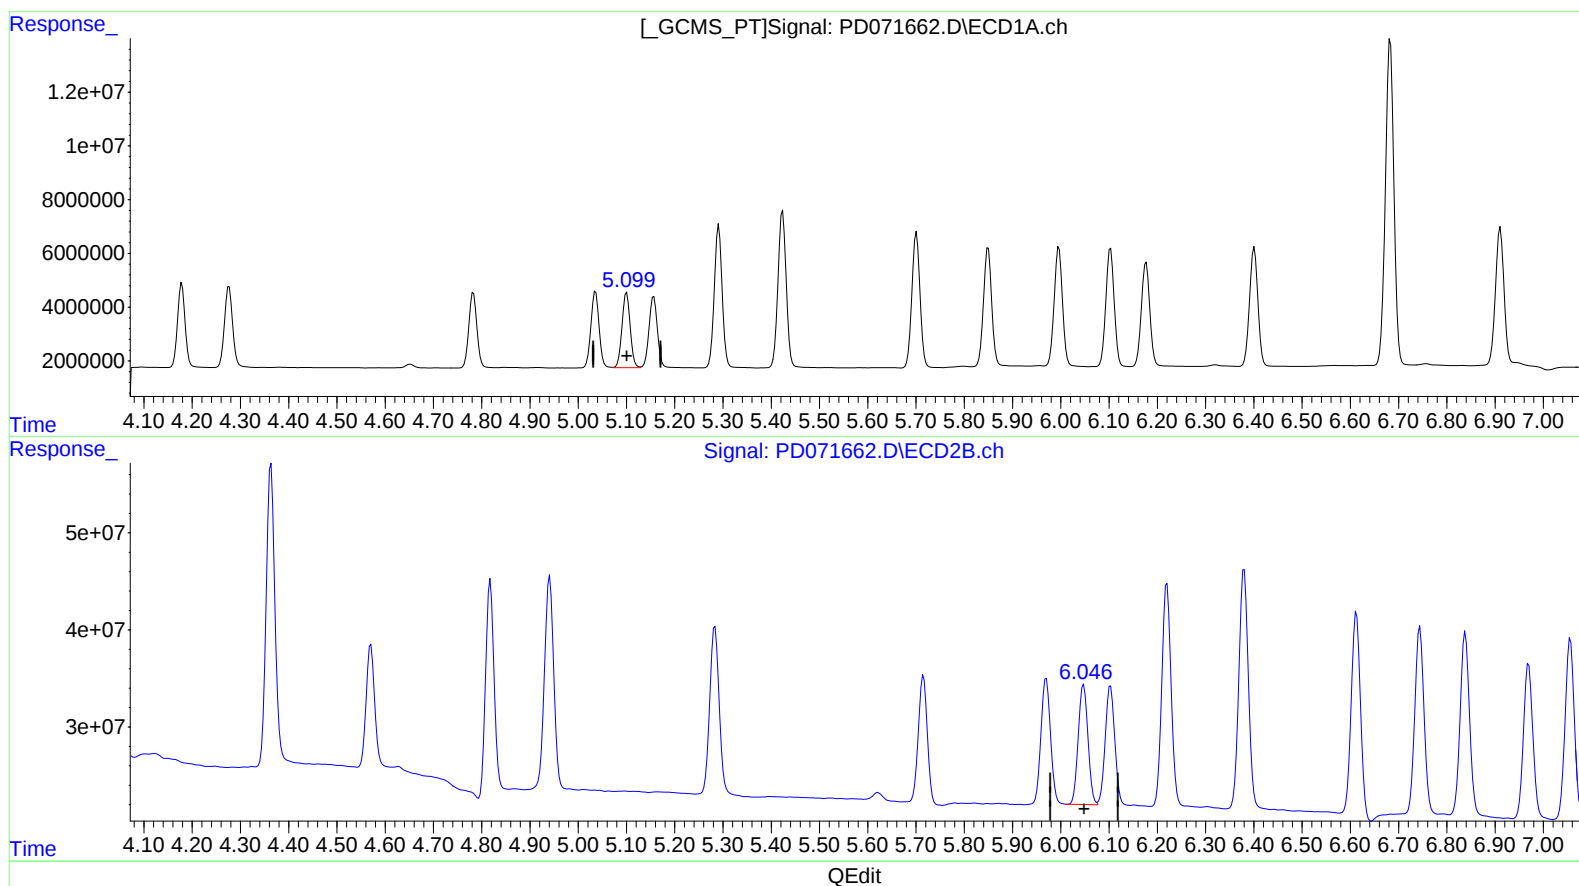

(11) cis-Chlordane (B)

5.101min 9.943 ng/ml

response 33163923

(11) cis-Chlordane #2 (B)

6.048min 10.503 ng/ml


response 171192051

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082622\
Data File : PD071662.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Aug 2022 16:29
Operator : AR\AJ
Sample : RESC036
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC038

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 02:00:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 27 07:11:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

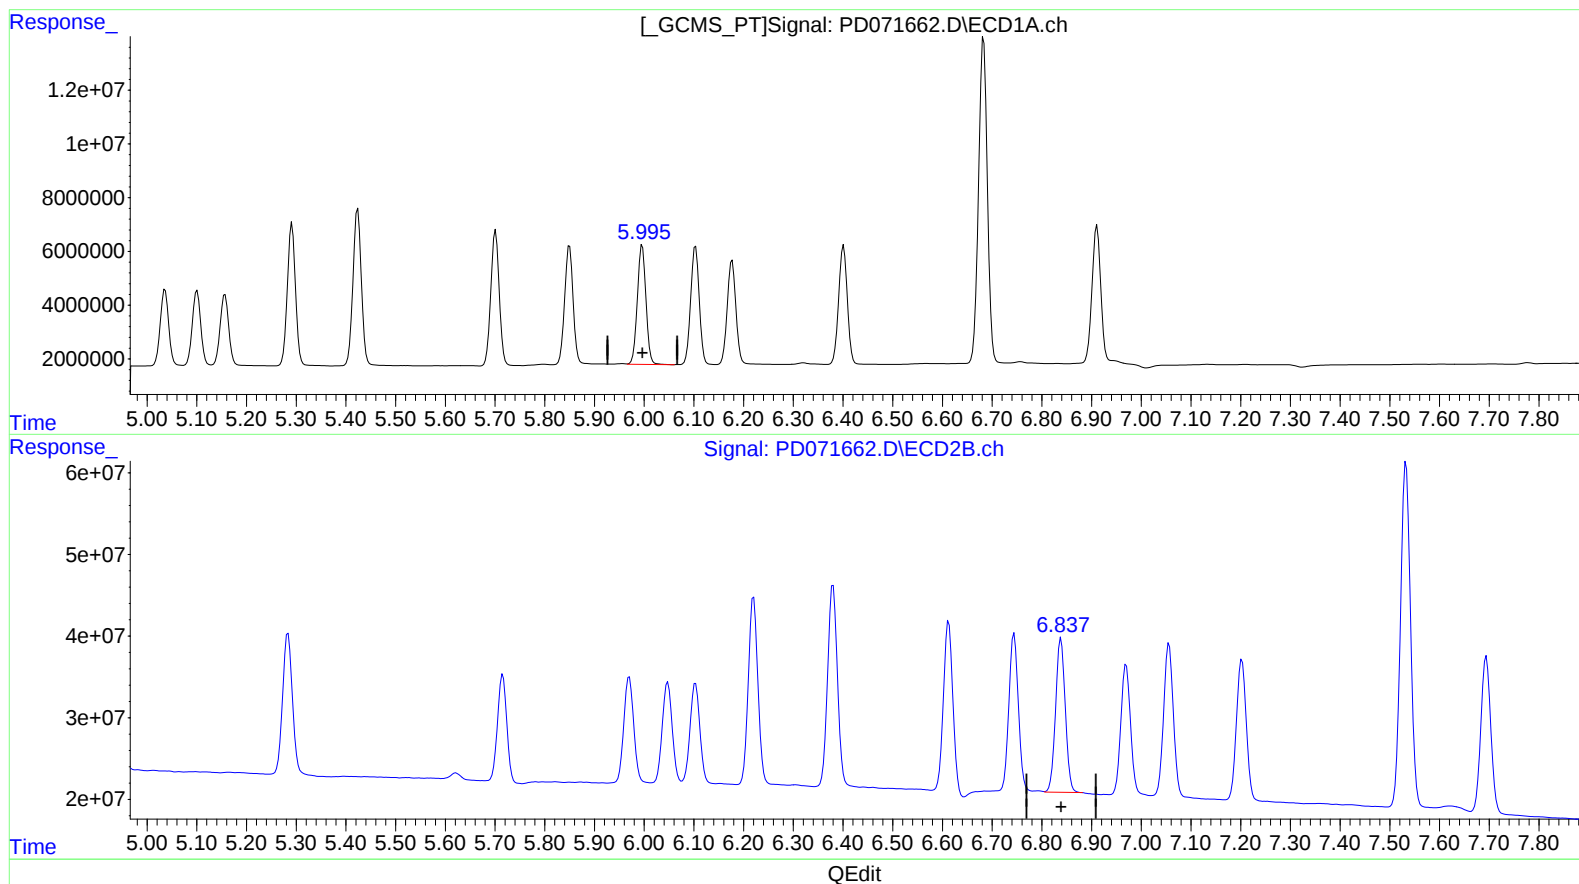

(15) Endosulfan II (B)
5.996min 20.039 ng/ml
response 53264843

(15) Endosulfan II #2 (B)
6.838min 21.189 ng/ml
response 255412414