

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082624\
 Data File : PD084669.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2024 10:24
 Operator : AR\AJ
 Sample : PB162826BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK826

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 06:55:07 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082424CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 03:41:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.906	20181993	69534595	21.144	20.600
27)	SA Decachlor...	9.034	8.108	33409631	88646999	27.731	26.728
Target Compounds							
2)	A alpha-BHC	0.000	3.411	0	207979	N.D.	<MDL
3)	MA gamma-BHC...	0.000	3.754	0	452641	N.D.	<MDL
4)	MA Heptachlor	0.000	4.135f	0	71068	N.D.	<MDL
5)	MB Aldrin	0.000	4.422f	0	79226	N.D.	<MDL
7)	B delta-BHC	4.761	4.291	1045348	140570	0.637	<MDL #
8)	B Heptachlo...	0.000	4.906	0	84932	N.D.	<MDL
9)	A Endosulfan I	0.000	5.310f	0	121548	N.D.	<MDL
10)	B trans-Chl...	0.000	5.139	0	79629	N.D.	<MDL
11)	B cis-Chlor...	0.000	5.221	0	40409	N.D.	<MDL
12)	B 4,4'-DDE	6.127f	5.401	155609	1003	0.126	<MDL #
13)	MA Dieldrin	0.000	5.527	0	125339	N.D.	<MDL
14)	MA Endrin	0.000	5.825	0	568293	N.D.	0.156
15)	B Endosulfa...	0.000	6.064f	0	1140233	N.D.	0.322
16)	A 4,4'-DDD	0.000	5.958	0	72362	N.D.	<MDL
18)	B Endrin al...	0.000	6.299	0	178244	N.D.	<MDL
19)	B Endosulfa...	0.000	6.513	0	688134	N.D.	0.200
20)	A Methoxychlor	7.524f	6.793	2094578	147126	4.098	<MDL #
21)	B Endrin ke...	0.000	7.042	0	5817393	N.D.	1.377
22)	Toxaphene-1	0.000	5.182	0	218158	N.D.	9.022
23)	Toxaphene-2	0.000	5.527	0	125339	N.D.	5.154
24)	Toxaphene-3	0.000	6.793	0	147126	N.D.	1.830
26)	Toxaphene-5	0.000	7.326f	0	372303	N.D.	9.379


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082624\
Data File : PD084669.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2024 10:24
Operator : AR\AJ
Sample : PB162826BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 06:55:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082424CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 03:41:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

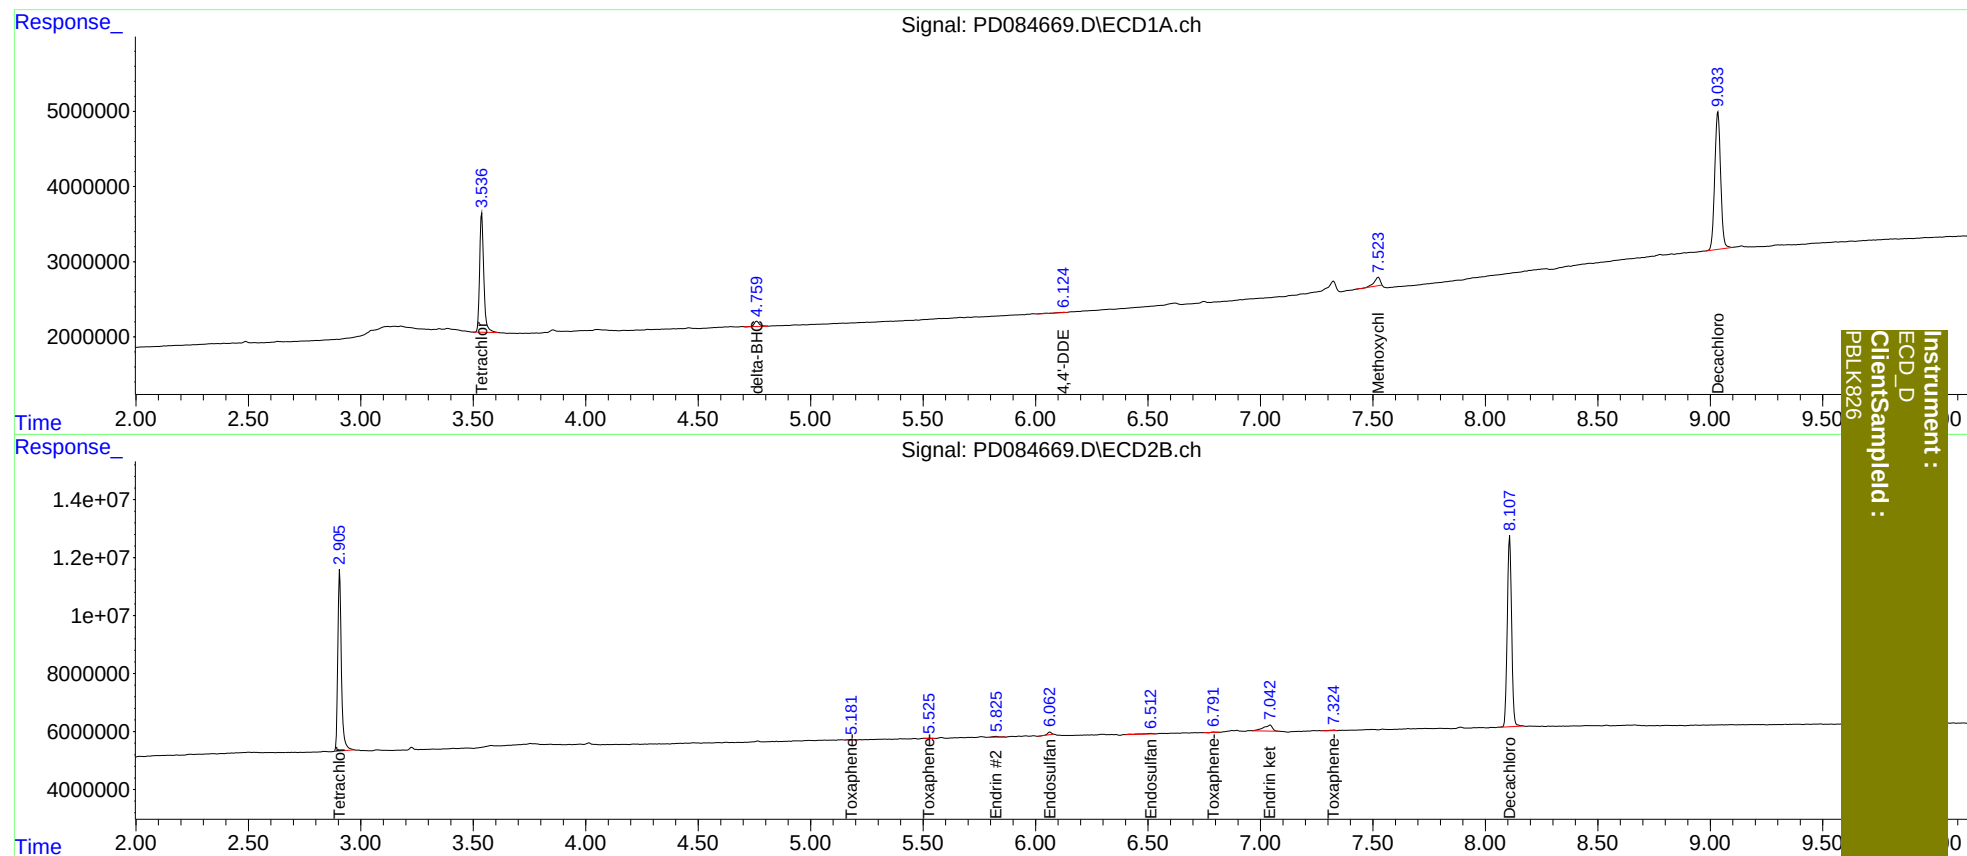


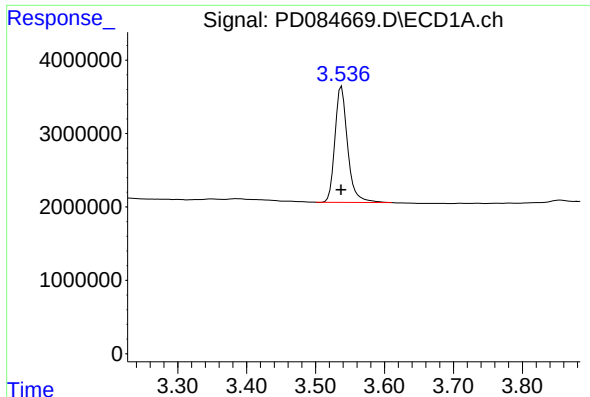

#1 Tetrachloro-m-xylene


R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 20181993
Conc: 21.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK826

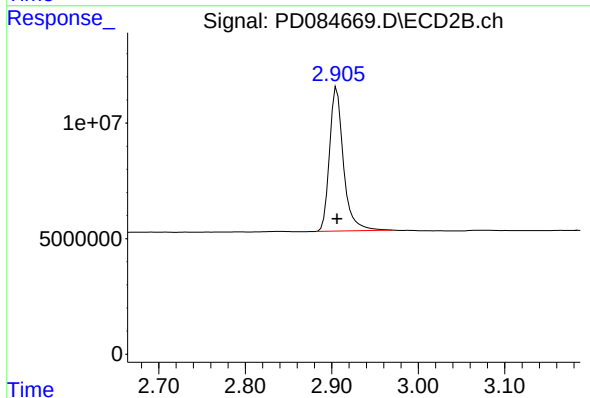


#1 Tetrachloro-m-xylene

R.T.: 2.906 min
Delta R.T.: 0.000 min
Response: 69534595
Conc: 20.60 ng/ml

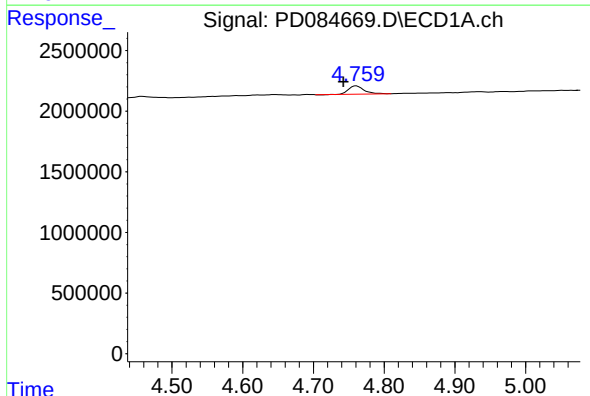


#7 delta-BHC

R.T.: 4.761 min
Delta R.T.: 0.018 min
Response: 1045348
Conc: 0.64 ng/ml

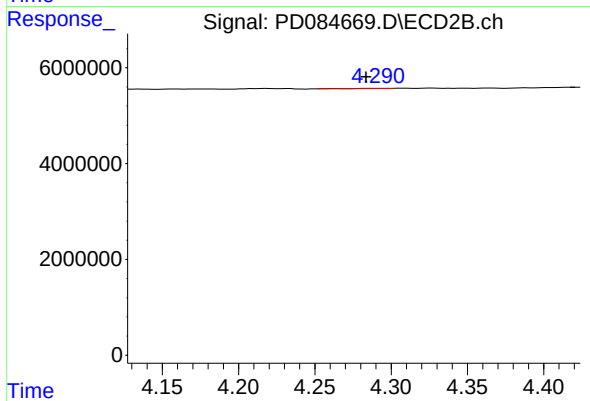

#7 delta-BHC


R.T.: 4.291 min
Delta R.T.: 0.007 min
Response: 140570
Conc: N.D.

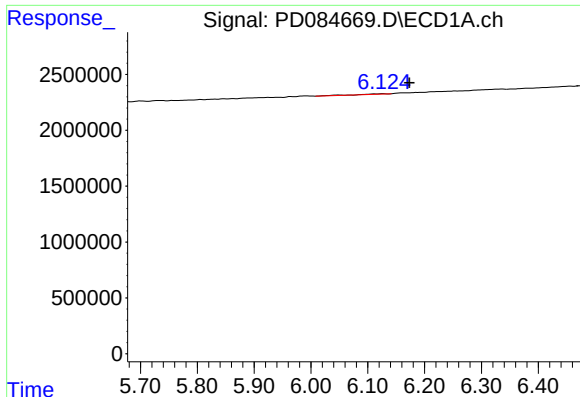

#12 4,4'-DDE


R.T.: 6.127 min
Delta R.T.: -0.047 min
Response: 155609
Conc: 0.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK826

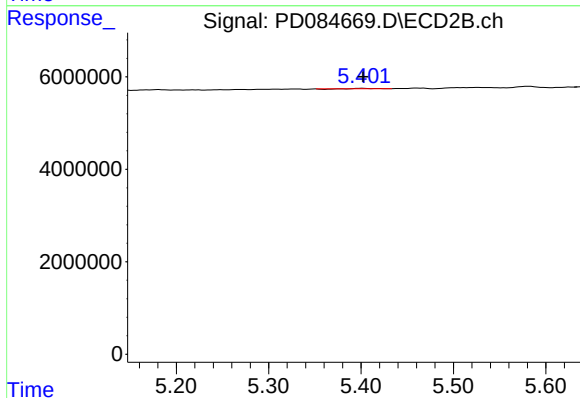


#12 4,4'-DDE

R.T.: 5.401 min
Delta R.T.: -0.001 min
Response: 1003
Conc: N.D.

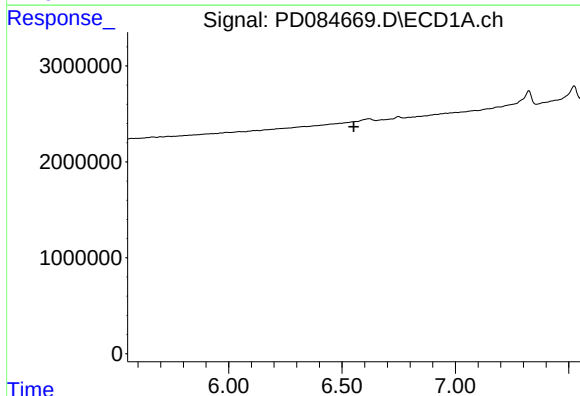


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.551 min
Response: 0
Conc: N.D.

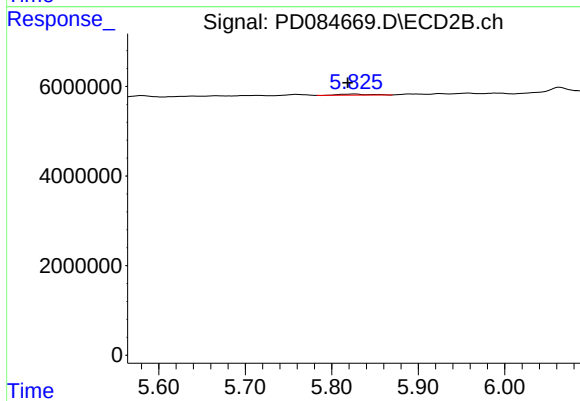

#14 Endrin


R.T.: 5.825 min
Delta R.T.: 0.006 min
Response: 568293
Conc: 0.16 ng/ml

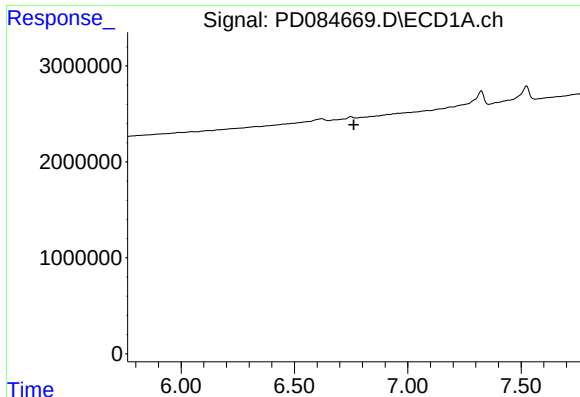

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.762 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PBLK826

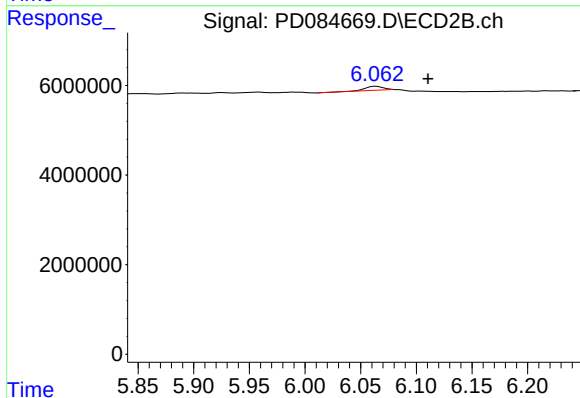


#15 Endosulfan II

R.T.: 6.064 min
Delta R.T.: -0.046 min
Response: 1140233
Conc: 0.32 ng/ml

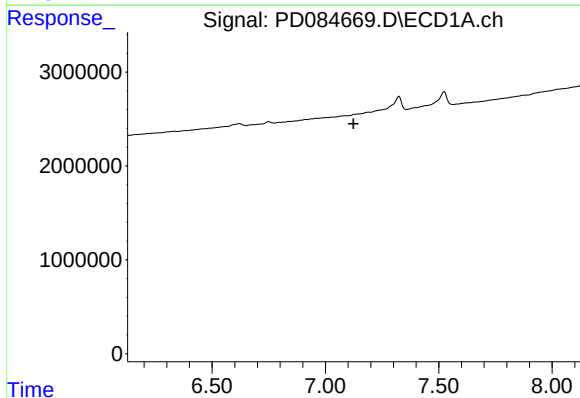


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 7.124 min
Response: 0
Conc: N.D.

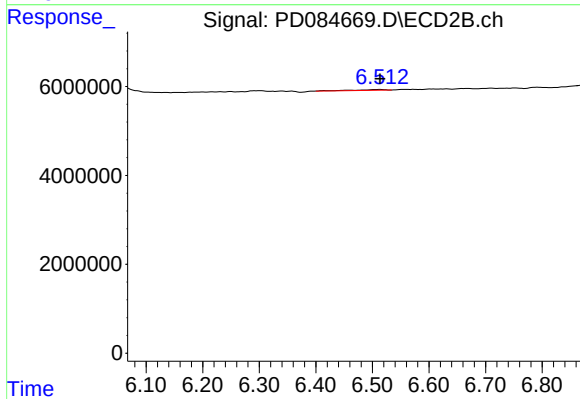

#19 Endosulfan Sulfate


R.T.: 6.513 min
Delta R.T.: 0.000 min
Response: 688134
Conc: 0.20 ng/ml

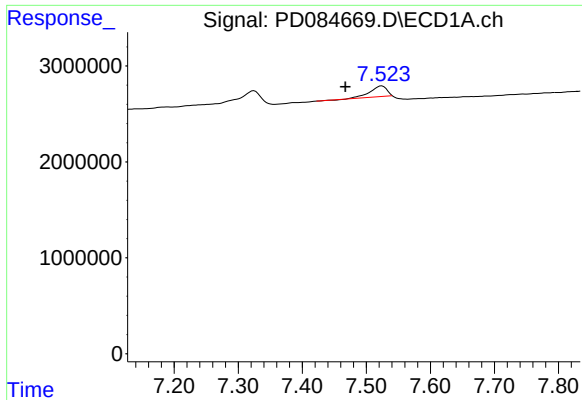

#20 Methoxychlor


R.T.: 7.524 min
Delta R.T.: 0.056 min
Response: 2094578
Conc: 4.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK826

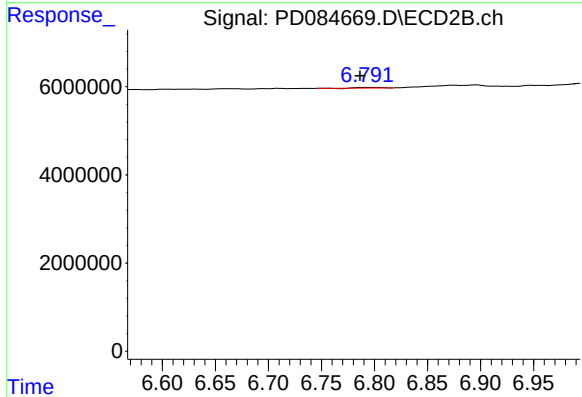


#20 Methoxychlor

R.T.: 6.793 min
Delta R.T.: 0.007 min
Response: 147126
Conc: N.D.

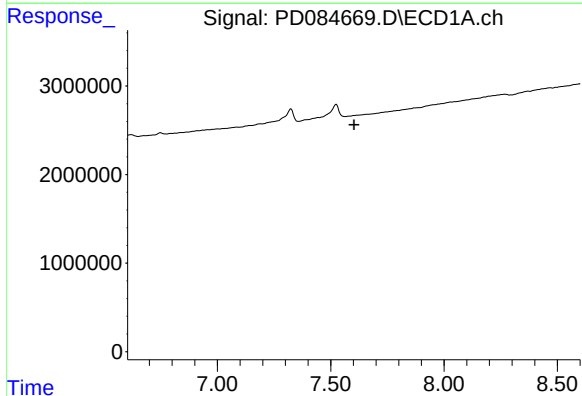


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.604 min
Response: 0
Conc: N.D.

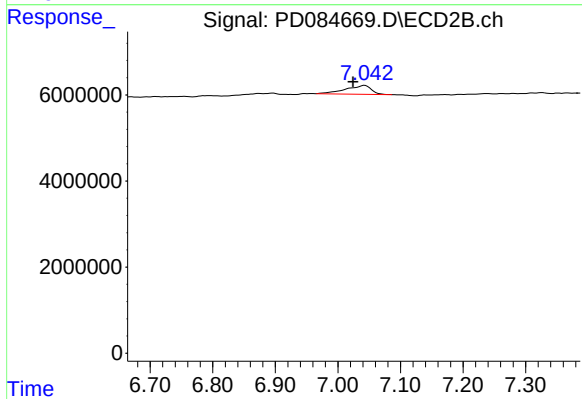

#21 Endrin ketone


R.T.: 7.042 min
Delta R.T.: 0.018 min
Response: 5817393
Conc: 1.38 ng/ml

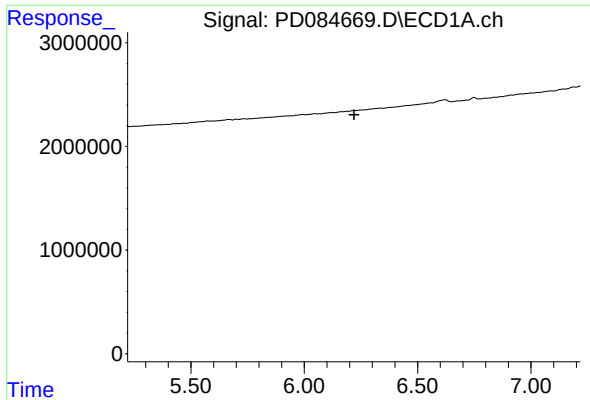

#22 Toxaphene-1


R.T.: 0.000 min
Exp R.T.: 6.220 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PBLK826

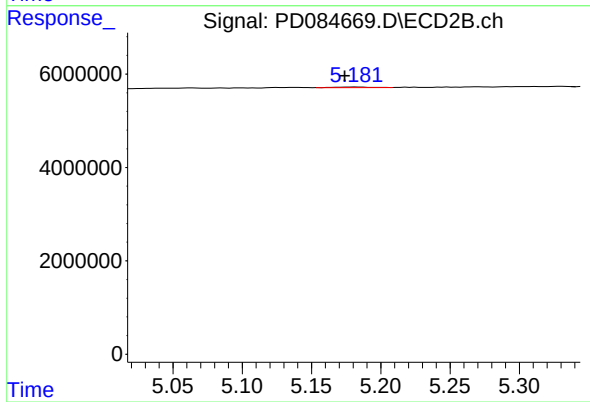


#22 Toxaphene-1

R.T.: 5.182 min
Delta R.T.: 0.008 min
Response: 218158
Conc: 9.02 ng/ml

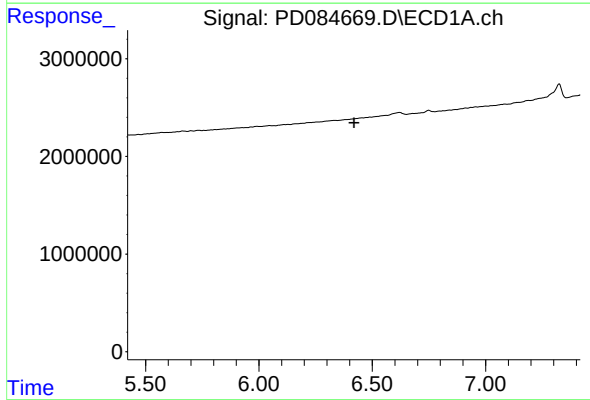


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T.: 6.420 min
Response: 0
Conc: N.D.

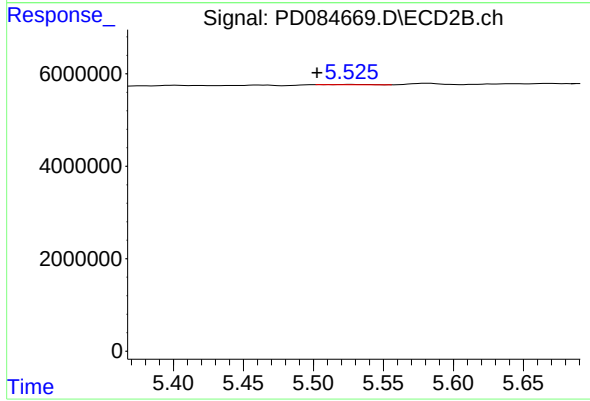

#23 Toxaphene-2


R.T.: 5.527 min
Delta R.T.: 0.025 min
Response: 125339
Conc: 5.15 ng/ml

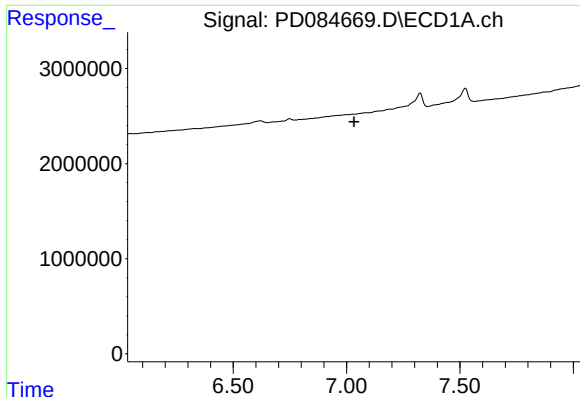

#24 Toxaphene-3


R.T.: 0.000 min
Exp R.T.: 7.033 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PBLK826

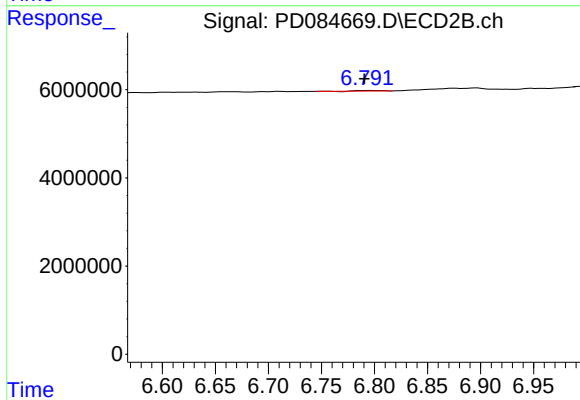


#24 Toxaphene-3

R.T.: 6.793 min
Delta R.T.: 0.003 min
Response: 147126
Conc: 1.83 ng/ml

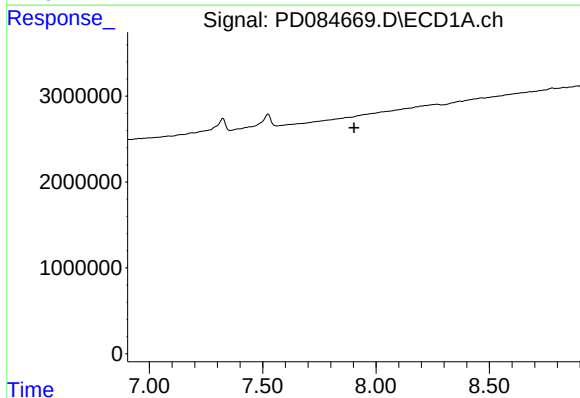


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T.: 7.904 min
Response: 0
Conc: N.D.

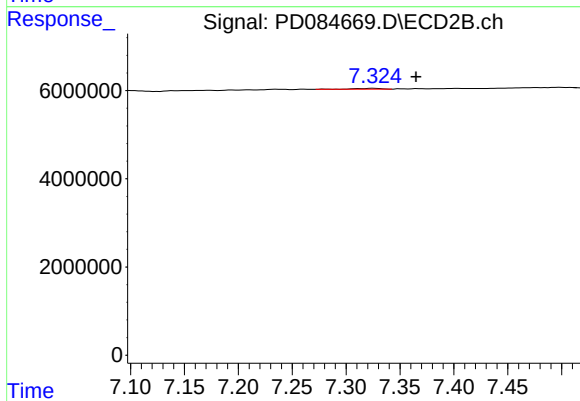

#26 Toxaphene-5

R.T.: 7.326 min
Delta R.T.: -0.039 min
Response: 372303
Conc: 9.38 ng/ml

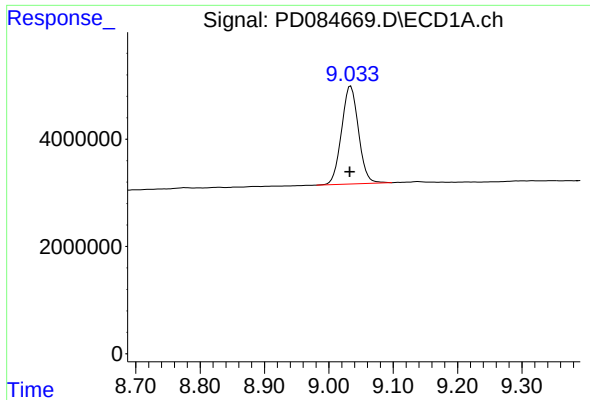

#27 Decachlorobiphenyl


R.T.: 9.034 min

Delta R.T.: 0.001 min

Response: 33409631

Conc: 27.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK826

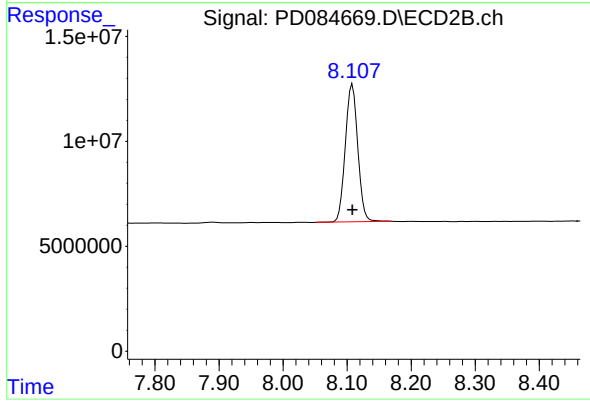

#27 Decachlorobiphenyl

R.T.: 8.108 min

Delta R.T.: 0.000 min

Response: 88646999

Conc: 26.73 ng/ml