

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082624\
 Data File : PD084670.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2024 10:37
 Operator : AR\AJ
 Sample : PB162826BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS826

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/28/2024
 Supervised By :Ankita Jodhani 08/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 06:55:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082424CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 03:41:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.906	18573235	64278467	19.458	19.043
27)	SA Decachlor...	9.033	8.108	31127557	82765274	25.837	24.955
Target Compounds							
2)	A alpha-BHC	3.983	3.417	6944464	23271743	4.087	4.582
3)	MA gamma-BHC...	4.312	3.752	7155025	23503713	4.449	4.891
4)	MA Heptachlor	4.910	4.107	7325193	20353090	4.843	4.852
5)	MB Aldrin	5.251	4.394	7172897	21163725	4.593	4.853
6)	B beta-BHC	4.493	4.044	3545936	10745112	5.087m	5.051m
7)	B delta-BHC	4.743	4.283	7580583	19552809	4.621	3.995
8)	B Heptachlo...	5.670	4.898	7031439	21032808	4.911	5.109
9)	A Endosulfan I	6.053	5.273	6660323	19336260	5.034	5.069m
10)	B trans-Chl...	5.924	5.152	6750620	20547602	4.962	5.122
11)	B cis-Chlor...	6.005	5.217	7088124	21036373	5.002	5.182
12)	B 4,4'-DDE	6.172	5.402	11435491	38419532	9.249m	10.001
13)	MA Dieldrin	6.325	5.541	13365410	42653764	9.292	10.112
14)	MA Endrin	6.552	5.818	10105077	37067205	9.178	10.175
15)	B Endosulfa...	6.762	6.110	12501455	38222810	9.941	10.804
16)	A 4,4'-DDD	6.682	5.958	9060795	34921621	9.579	10.590
17)	MA 4,4'-DDT	6.997	6.213	7419539	31161644	8.345	9.830
18)	B Endrin al...	6.891	6.289	9469556	30638195	11.361	11.492
19)	B Endosulfa...	7.124	6.513	10836818	35957364	9.882	10.475
20)	A Methoxychlor	7.467	6.786	24870970	85764833	48.658	53.788
21)	B Endrin ke...	7.604	7.024	12496071	51047812	10.725	12.086

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082624\
Data File : PD084670.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2024 10:37
Operator : AR\AJ
Sample : PB162826BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 06:55:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082424CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 03:41:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

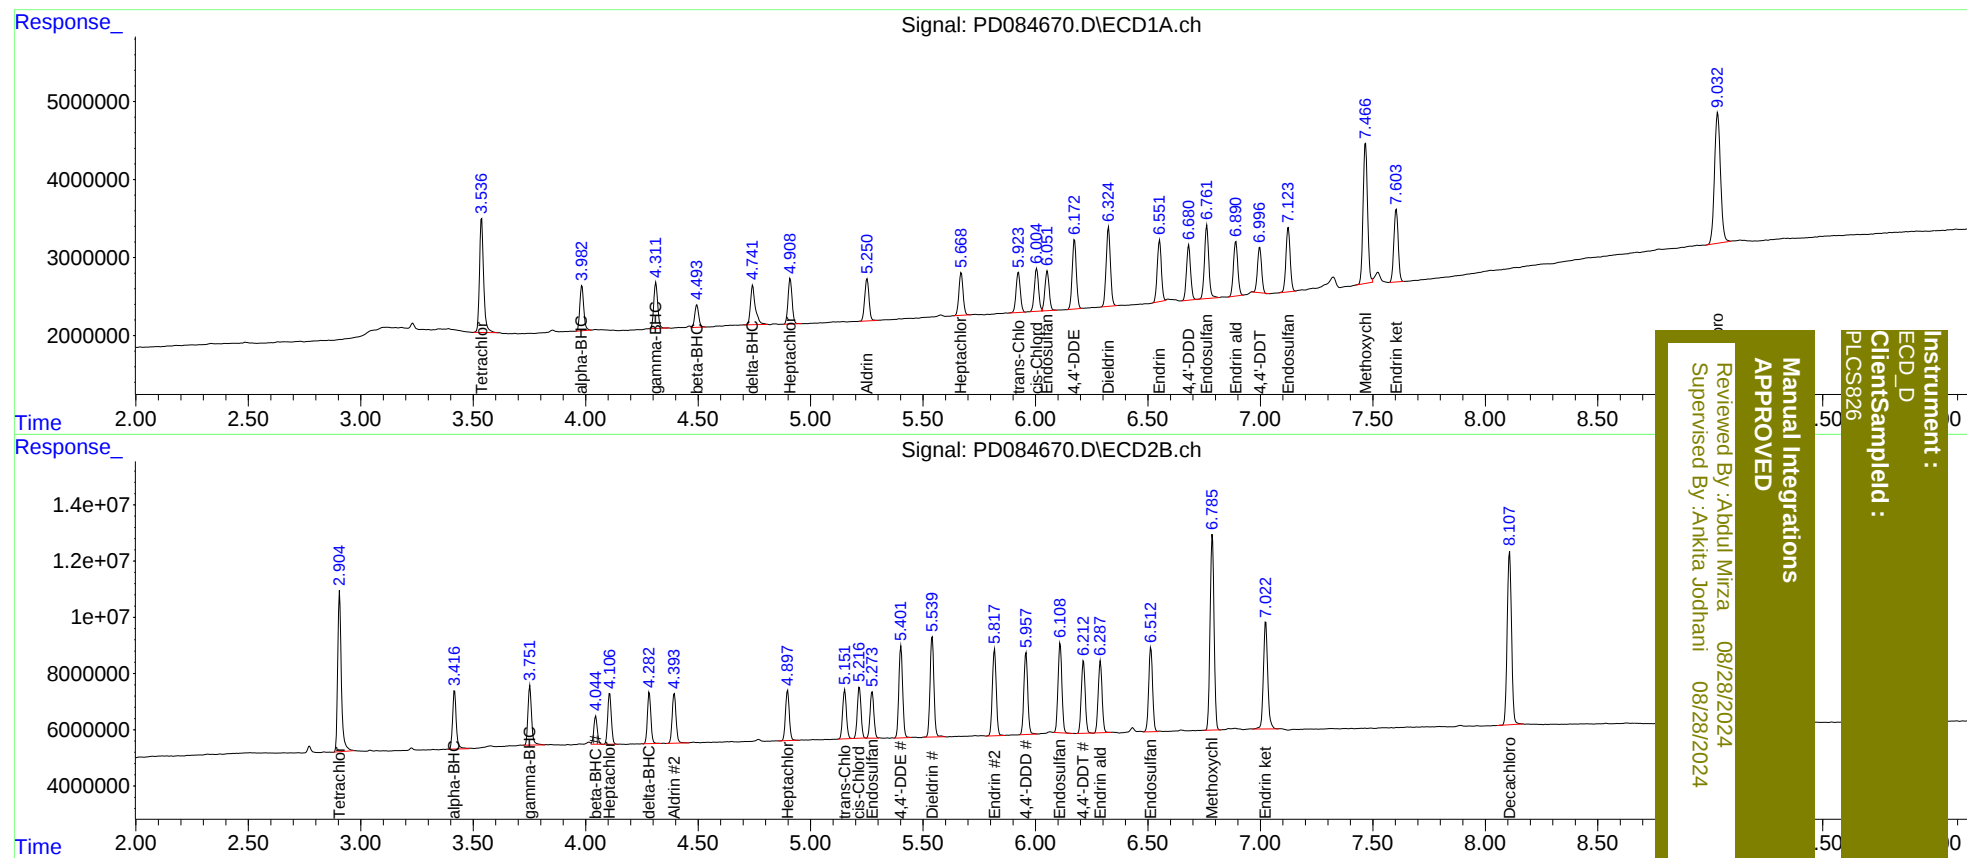

Reviewed By: Abdul Mirza 08/28/2024
Supervised By: Ankita Jodhani 08/28/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
PLCS826