

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082624\
 Data File : PD084671.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2024 10:50
 Operator : AR\AJ
 Sample : P3593-01 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCXW2

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/28/2024
 Supervised By :Ankita Jodhani 08/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 06:55:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082424CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 03:41:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.538	2.907	19161597	66965067	20.075	19.839
2) SA Decachlor...	9.033	8.108	25616613	68700633	21.262	20.714
Target Compounds						
6) B beta-BHC	4.496	4.047	592563	1949997	0.850	0.917m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082624\
Data File : PD084671.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2024 10:50
Operator : AR\AJ
Sample : P3593-01 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 06:55:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082424CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 03:41:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

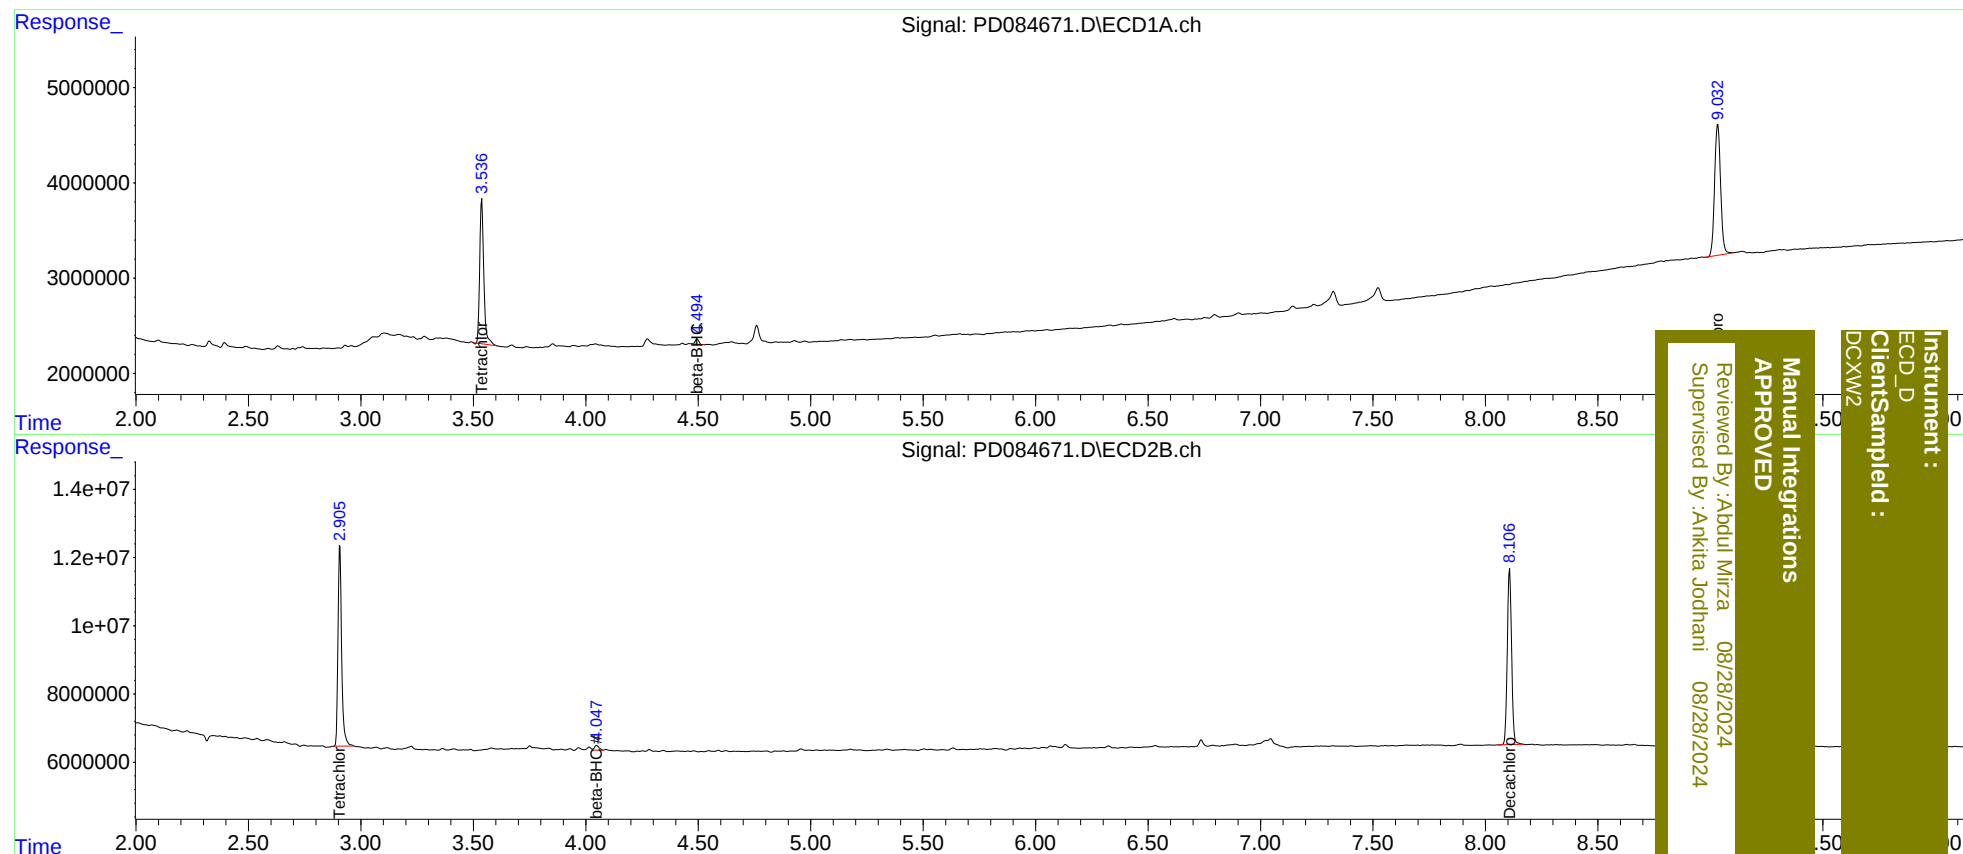

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 08/28/2024
Supervised By: Ankita Jodhani 08/28/2024

Instrument :
ECD_D
Client Sampled :
DCXM2