

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082724\
 Data File : PD084687.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2024 14:31
 Operator : AR\AJ
 Sample : P3626-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCYE9

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 05:35:07 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.906	8378508	30025836	8.284	8.485
27)	SA Decachlor...	9.036	8.109	3241529	42120709	2.482	12.113 #
Target Compounds							
8)	B Heptachlo...	0.000	4.897	0	33305588	N.D.	7.864
9)	A Endosulfan I	6.004f	5.295	15793258	26440223	11.479	6.898 #
10)	B trans-Chl...	5.914	0.000	11017180	0	7.812	N.D. #
11)	B cis-Chlor...	6.004	0.000	15793258	0	10.682	N.D. #
12)	B 4,4'-DDE	0.000	5.437	0	18906403	N.D.	4.820
13)	MA Dieldrin	6.277f	0.000	5572123	0	3.777	N.D. #
22)	Toxaphene-1	5.830	0.000	106932	0	25.370	N.D. #
23)	Toxaphene-2	6.463f	5.437f	2793021	18906403	189.893	764.921 #
26)	Toxaphene-5	7.936	0.000	1405410	0	74.600	N.D. #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082724\
Data File : PD084687.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2024 14:31
Operator : AR\AJ
Sample : P3626-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 05:35:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

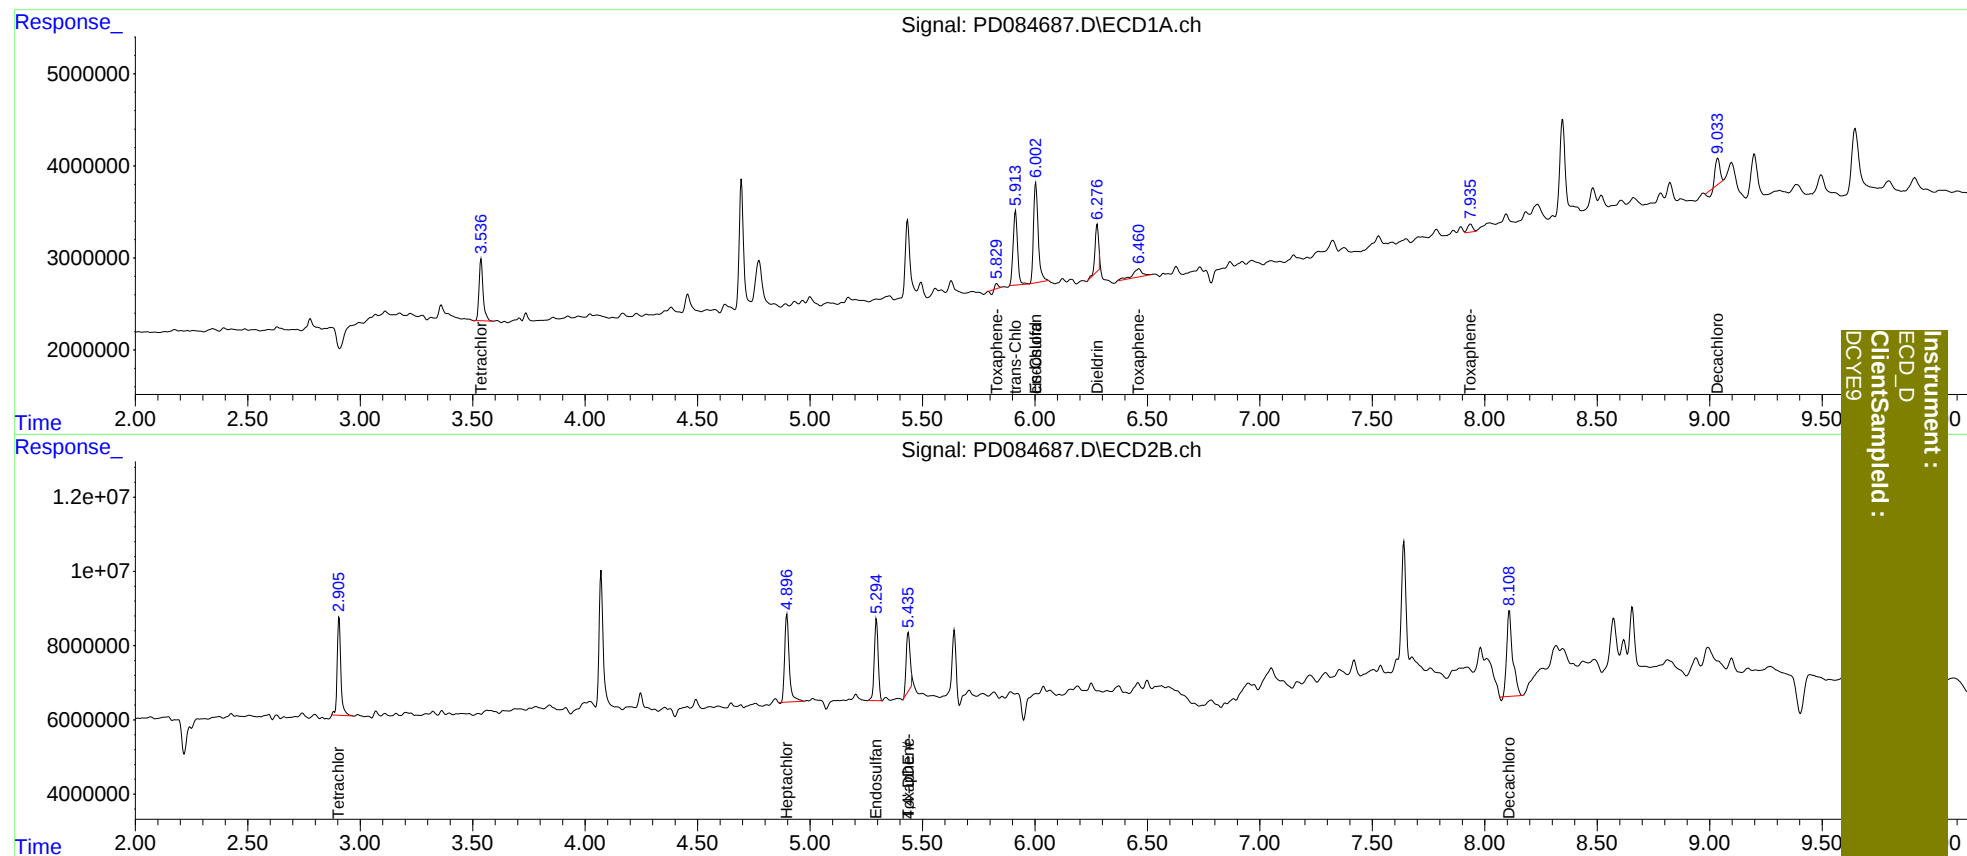

The printer must be in Portrait mode.

Instrument :
ECD_D
ClientSampleId :
DCYE9