

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082724\
 Data File : PD084690.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2024 15:11
 Operator : AR\AJ
 Sample : P3626-10MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCYB8MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 05:35:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.906	12880315	43857084	12.735	12.393
27)	SA Decachlor...	9.035	8.109	14856572	39508433	11.375	11.362
Target Compounds							
2)	A alpha-BHC	3.984	3.418	102.0E6	276.9E6	59.974	54.606
3)	MA gamma-BHC...	4.313	3.753	98191224	263.6E6	60.692	54.406
4)	MA Heptachlor	4.910	4.108	94280747	230.5E6	61.277	54.139
5)	MB Aldrin	5.252	4.394	94229418	208.2E6	58.917	46.881
6)	B beta-BHC	4.495	4.046	38221411	107.5E6	52.620	49.577
7)	B delta-BHC	4.743	4.284	96014668	266.0E6	58.545	53.579
8)	B Heptachlo...	5.671	4.899	80284795	219.5E6	53.829	51.818
9)	A Endosulfan I	6.053	5.275	26207229	172.2E6	19.049	44.927 #
10)	B trans-Chl...	5.925	5.153	81974289	219.4E6	58.122	53.337
11)	B cis-Chlor...	6.006	5.218	77800921	218.8E6	52.619	52.146
12)	B 4,4'-DDE	6.174	5.403	157.3E6	428.2E6	126.073	109.160
13)	MA Dieldrin	6.326	5.542	173.3E6	456.5E6	117.499	106.267
14)	MA Endrin	6.553	5.819	149.6E6	420.6E6	132.574	113.605
15)	B Endosulfa...	6.763	6.111	145.5E6	396.4E6	110.260	106.919
16)	A 4,4'-DDD	6.683	5.960	120.6E6	358.3E6	122.124	105.586
17)	MA 4,4'-DDT	6.999	6.215	111.8E6	366.5E6	124.897	114.557
18)	B Endrin al...	6.891	6.289	105.6E6	298.8E6	116.915	104.668
19)	B Endosulfa...	7.126	6.514	136.7E6	397.0E6	118.664	111.158
20)	A Methoxychlor	7.469	6.787	323.9E6	875.3E6	621.715	529.121
21)	B Endrin ke...	7.605	7.025	145.9E6	452.3E6	119.364	102.713
22)	Toxaphene-1	0.000	5.153	0	219.4E6	N.D.	8652.859
23)	Toxaphene-2	6.457f	5.542f	2130276	456.5E6	144.834	18470.851 #
24)	Toxaphene-3	6.999	5.819f	111.8E6	420.6E6	3263.096	17824.894 #
25)	Toxaphene-4	7.126	0.000	136.7E6	0	5312.696	N.D. #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082724\
Data File : PD084690.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2024 15:11
Operator : AR\AJ
Sample : P3626-10MS
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 05:35:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

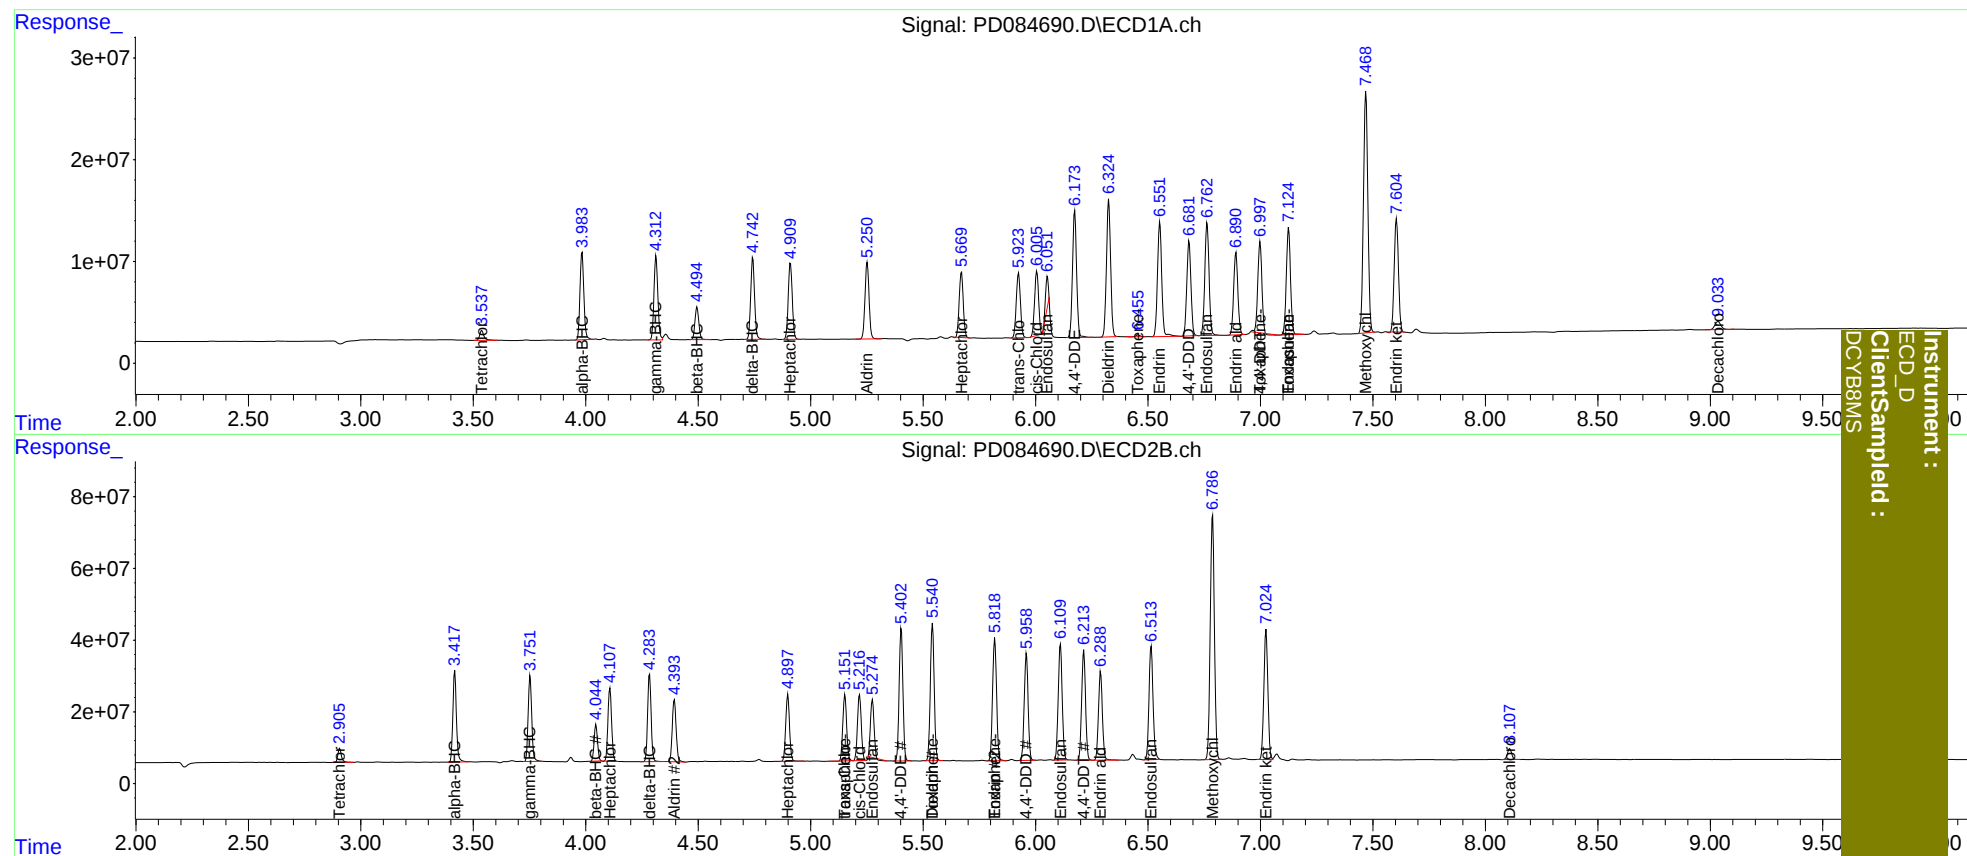

The printer must be in Portrait mode.

Instrument :
ECD_D
ClientSampleId :
DCYB8MS