

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082724\
 Data File : PD084691.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2024 15:24
 Operator : AR\AJ
 Sample : P3626-11MSD
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCYB8MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 05:35:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.906	13143508	43941113	12.995	12.417
27)	SA Decachlor...	9.035	8.108	15015352	40336716	11.497	11.600
Target Compounds							
2)	A alpha-BHC	3.983	3.418	103.9E6	280.1E6	61.136	55.253
3)	MA gamma-BHC...	4.312	3.752	99887136	268.2E6	61.740	55.345
4)	MA Heptachlor	4.910	4.108	96271999	234.1E6	62.571	54.997
5)	MB Aldrin	5.251	4.394	96015102	211.3E6	60.034	47.570
6)	B beta-BHC	4.495	4.045	38724609	108.9E6	53.312	50.229
7)	B delta-BHC	4.743	4.283	98899008	270.0E6	60.304	54.389
8)	B Heptachlo...	5.670	4.898	81261627	221.1E6	54.484	52.196
9)	A Endosulfan I	6.053	5.275	30580564	166.6E6	22.227	43.472 #
10)	B trans-Chl...	5.924	5.152	83462538	221.6E6	59.177	53.879
11)	B cis-Chlor...	6.006	5.217	79090672	221.9E6	53.492	52.885
12)	B 4,4'-DDE	6.174	5.403	160.6E6	434.7E6	128.715	110.822
13)	MA Dieldrin	6.325	5.541	177.3E6	463.4E6	120.191	107.866
14)	MA Endrin	6.552	5.819	153.1E6	426.5E6	135.692	115.186
15)	B Endosulfa...	6.763	6.111	149.4E6	401.1E6	113.191	108.175
16)	A 4,4'-DDD	6.682	5.959	123.4E6	363.1E6	125.006	106.986
17)	MA 4,4'-DDT	6.998	6.215	116.4E6	372.6E6	130.012	116.484
18)	B Endrin al...	6.891	6.290	107.1E6	303.7E6	118.606	106.352
19)	B Endosulfa...	7.125	6.514	139.4E6	403.1E6	121.027	112.865
20)	A Methoxychlor	7.468	6.787	330.0E6	889.0E6	633.409	537.374
21)	B Endrin ke...	7.605	7.025	148.8E6	459.1E6	121.722	104.262
22)	Toxaphene-1	0.000	5.152	0	221.6E6	N.D.	8740.794
23)	Toxaphene-2	6.457f	5.541f	1801107	463.4E6	122.454	18748.668 #
24)	Toxaphene-3	6.998	5.819f	116.4E6	426.5E6	3396.737	18072.963 #
25)	Toxaphene-4	7.125	0.000	139.4E6	0	5418.463	N.D. #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082724\
Data File : PD084691.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2024 15:24
Operator : AR\AJ
Sample : P3626-11MSD
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 05:35:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

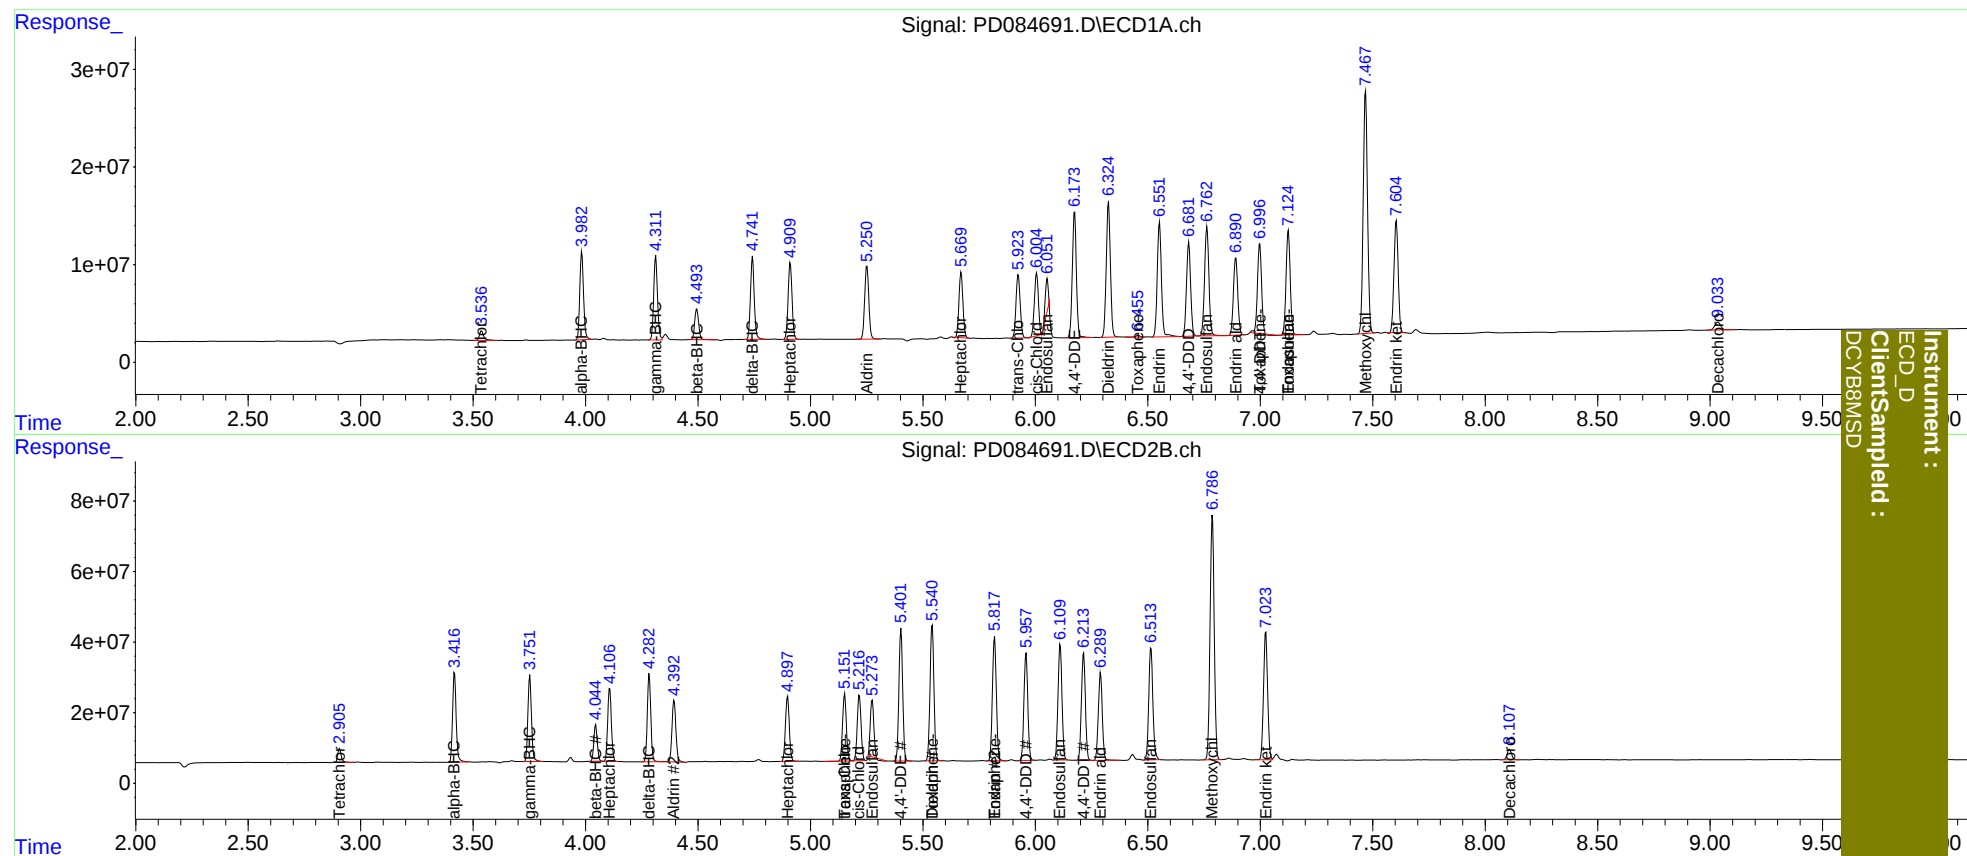

The printer must be in Portrait mode.

Instrument :
ECD_D
ClientSampleId :
DCYB8MSD