

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082724\
 Data File : PD084698.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2024 17:02
 Operator : AR\AJ
 Sample : P3626-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCYE1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 05:38:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.906	8516044	27817572	8.420	7.861
27)	SA Decachlor...	9.032	8.107	9357125	24494814	7.165	7.044
Target Compounds							
8)	B Heptachlo...	5.611f	0.000	8207529	0	5.503	N.D. #
10)	B trans-Chl...	0.000	5.129	0	11921746	N.D.	2.898
12)	B 4,4'-DDE	6.212f	0.000	1748279	0	1.401	N.D. #
19)	B Endosulfa...	0.000	6.532	0	320.3E6	N.D.	89.688
22)	Toxaphene-1	0.000	5.129f	0	11921746	N.D.	470.216

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082724\
Data File : PD084698.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2024 17:02
Operator : AR\AJ
Sample : P3626-15
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 05:38:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

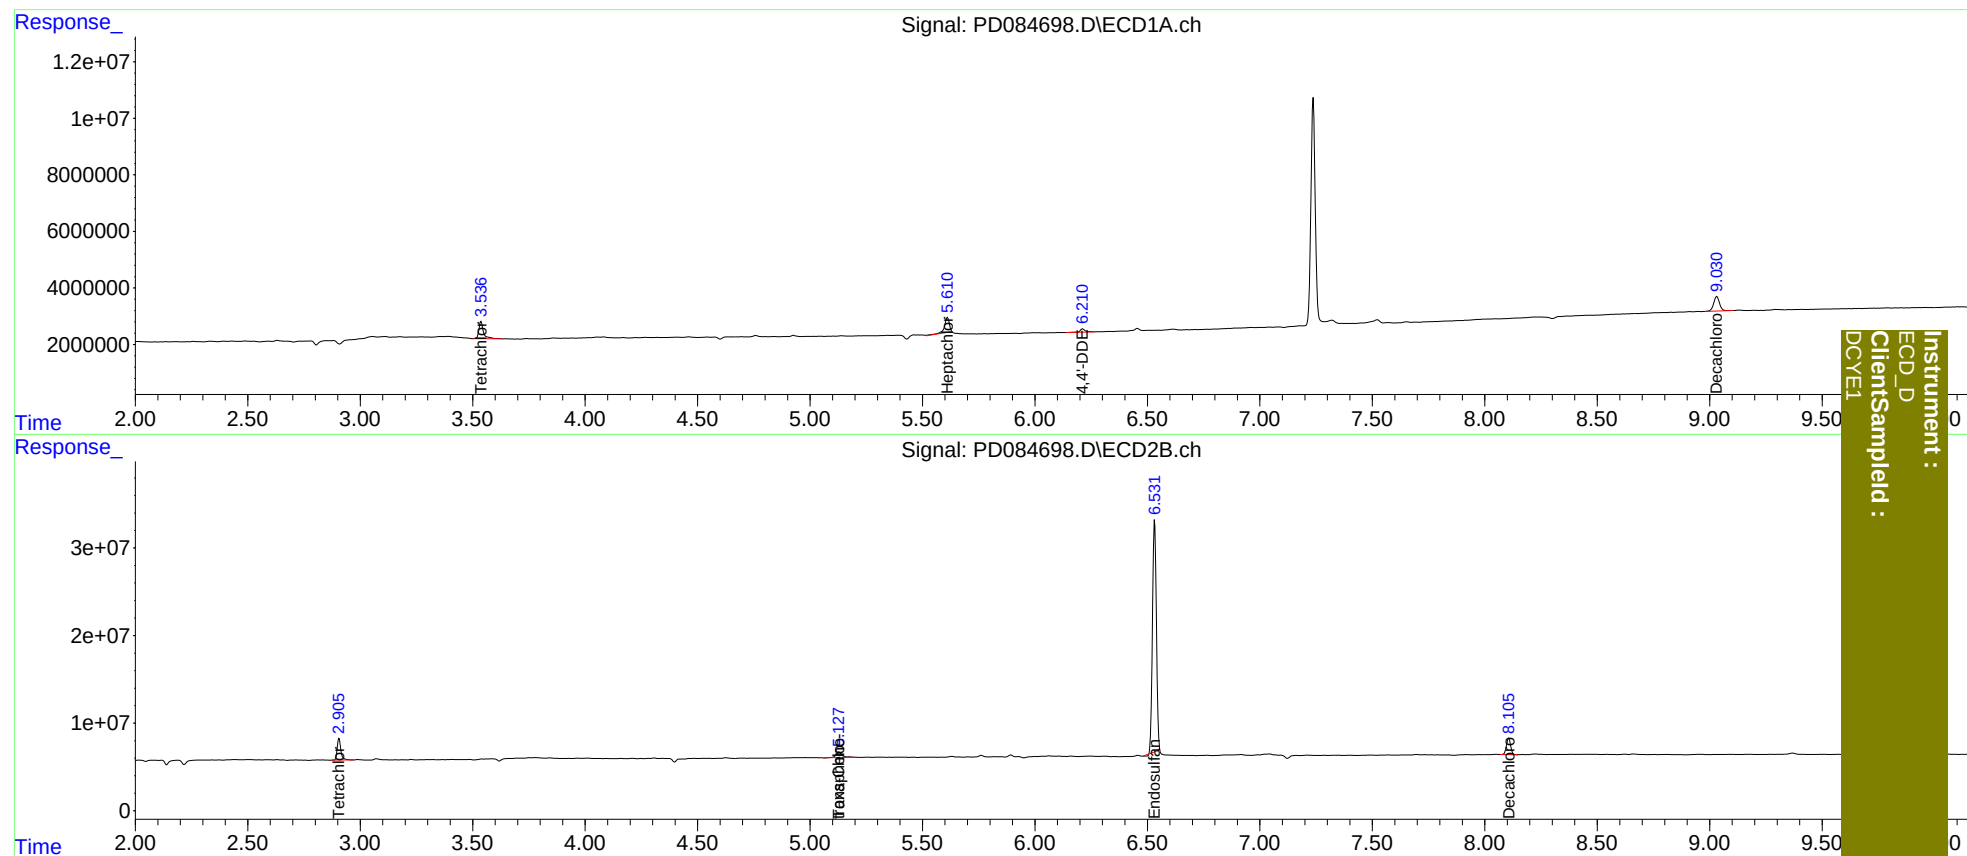

The printer must be in Portrait mode.

Instrument :
ECD_D
ClientSampleId :
DCYE1