

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082724\
 Data File : PD084700.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2024 17:29
 Operator : AR\AJ
 Sample : P3626-17
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCXZ5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 05:39:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.906	10005062	24739563	9.892	6.991 #
27)	SA Decachlor...	9.032	8.108	11759740	45992406	9.004	13.227 #
Target Compounds							
3)	MA gamma-BHC...	4.356f	0.000	53189880	0	32.877	N.D. #
5)	MB Aldrin	0.000	4.441f	0	10241127	N.D.	2.306
7)	B delta-BHC	4.771f	0.000	3537365	0	2.157	N.D. #
8)	B Heptachlo...	0.000	4.895	0	37893848	N.D.	8.947
9)	A Endosulfan I	6.002f	5.294	18536048	37008000	13.473	9.654 #
10)	B trans-Chl...	5.911	0.000	12480176	0	8.849	N.D. #
11)	B cis-Chlor...	6.002	0.000	18536048	0	12.537	N.D. #
12)	B 4,4'-DDE	0.000	5.436	0	27229535	N.D.	6.942
13)	MA Dieldrin	6.275f	0.000	635529	0	0.431	N.D. #
14)	MA Endrin	6.565	0.000	2224440	0	1.971	N.D. #
15)	B Endosulfa...	6.805f	0.000	660141	0	0.500	N.D. #
16)	A 4,4'-DDD	6.626f	0.000	1239980	0	1.256	N.D. #
17)	MA 4,4'-DDT	7.052f	0.000	2543374	0	2.841	N.D. #
19)	B Endosulfa...	7.149	0.000	5790117	0	5.026	N.D. #
21)	B Endrin ke...	7.584	7.054	3312283	34047929	2.709	7.733 #
23)	Toxaphene-2	0.000	5.436f	0	27229535	N.D.	1101.662
24)	Toxaphene-3	7.052	0.000	2543374	0	74.234	N.D. #
25)	Toxaphene-4	7.149	0.000	5790117	0	225.023	N.D. #
26)	Toxaphene-5	7.894	0.000	1985913	0	105.414	N.D. #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082724\
Data File : PD084700.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2024 17:29
Operator : AR\AJ
Sample : P3626-17
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 05:39:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

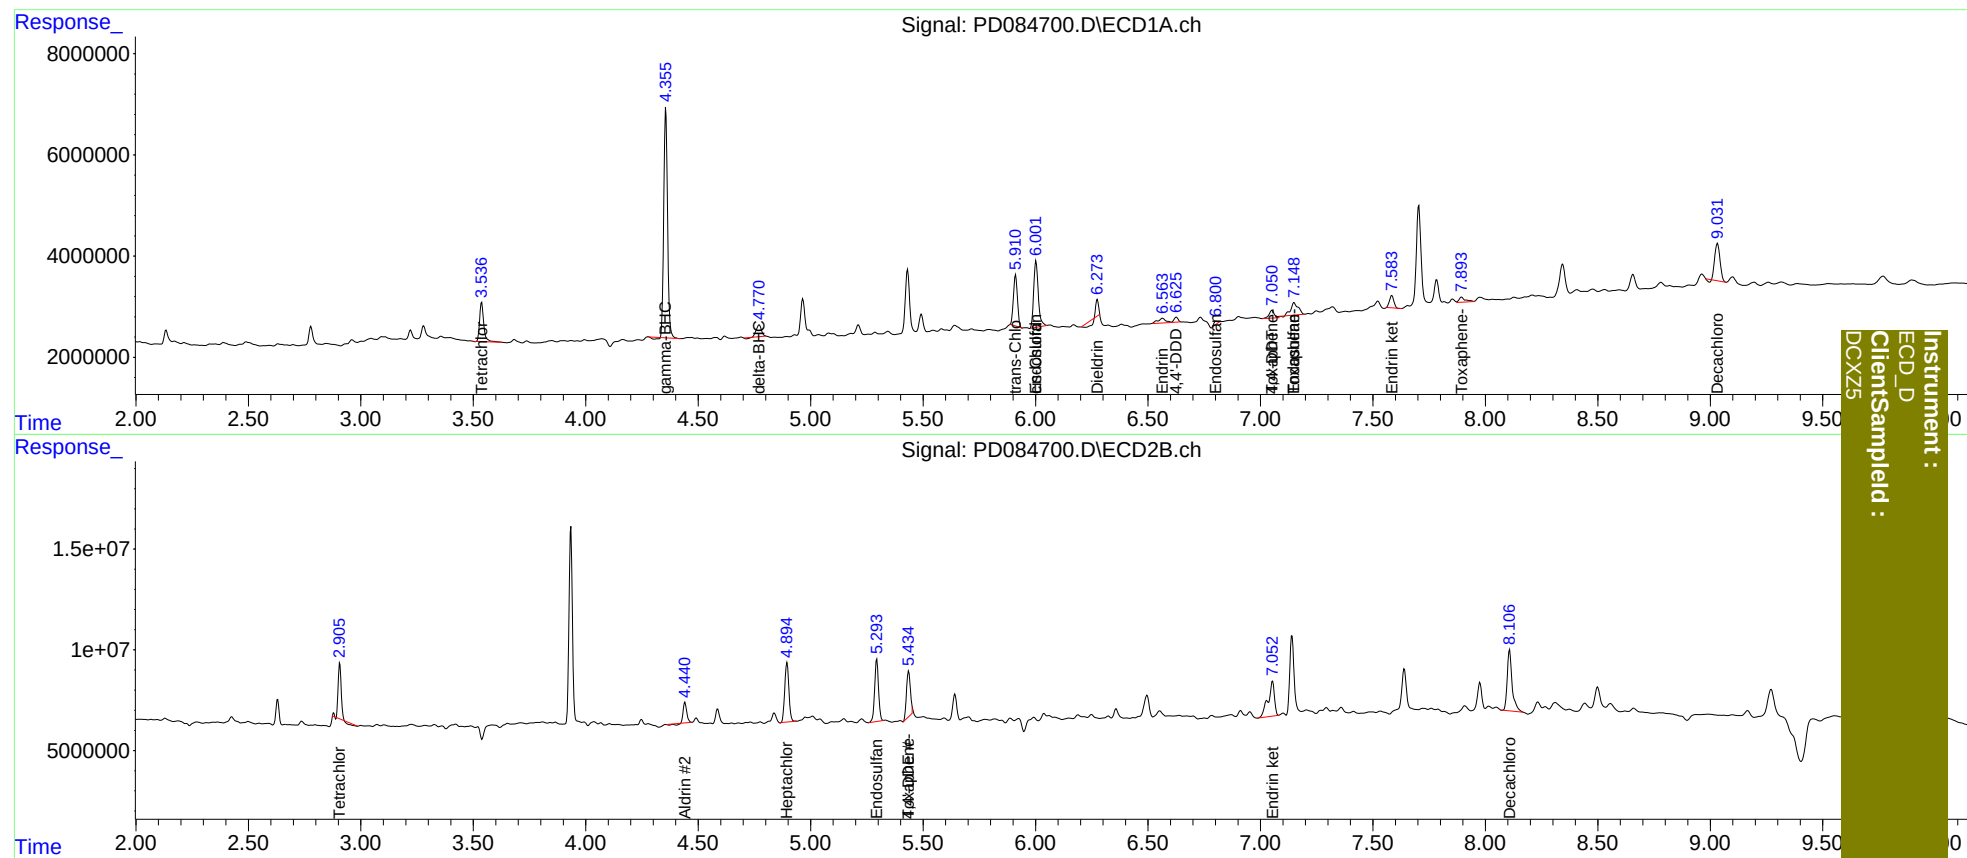

The printer must be in Portrait mode.

Instrument :
ECD_D
ClientSampleId :
DCXZ5