

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082724\
 Data File : PD084701.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2024 17:43
 Operator : AR\AJ
 Sample : P3626-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCXZ7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 05:39:14 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.906	14343107	50041619	14.181	14.141
27)	SA Decachlor...	9.032	8.107	20479402	51434918	15.681	14.792
Target Compounds							
3)	MA gamma-BHC...	4.356f	0.000	23012719	0	14.224	N.D. #
7)	B delta-BHC	4.765	0.000	1449331	0	0.884	N.D. #
14)	MA Endrin	6.508f	0.000	374826	0	0.332	N.D. #
19)	B Endosulfa...	7.151	0.000	3378180	0	2.932	N.D. #
20)	A Methoxychlor	7.530f	0.000	1809416	0	3.474	N.D. #
21)	B Endrin ke...	7.583	7.030	1973218	15192368	1.614	3.450 #
23)	Toxaphene-2	6.458f	0.000	87040	0	5.918	N.D. #
25)	Toxaphene-4	7.151	0.000	3378180	0	131.287	N.D. #
26)	Toxaphene-5	7.948f	0.000	1867423	0	99.124	N.D. #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082724\
Data File : PD084701.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2024 17:43
Operator : AR\AJ
Sample : P3626-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 05:39:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

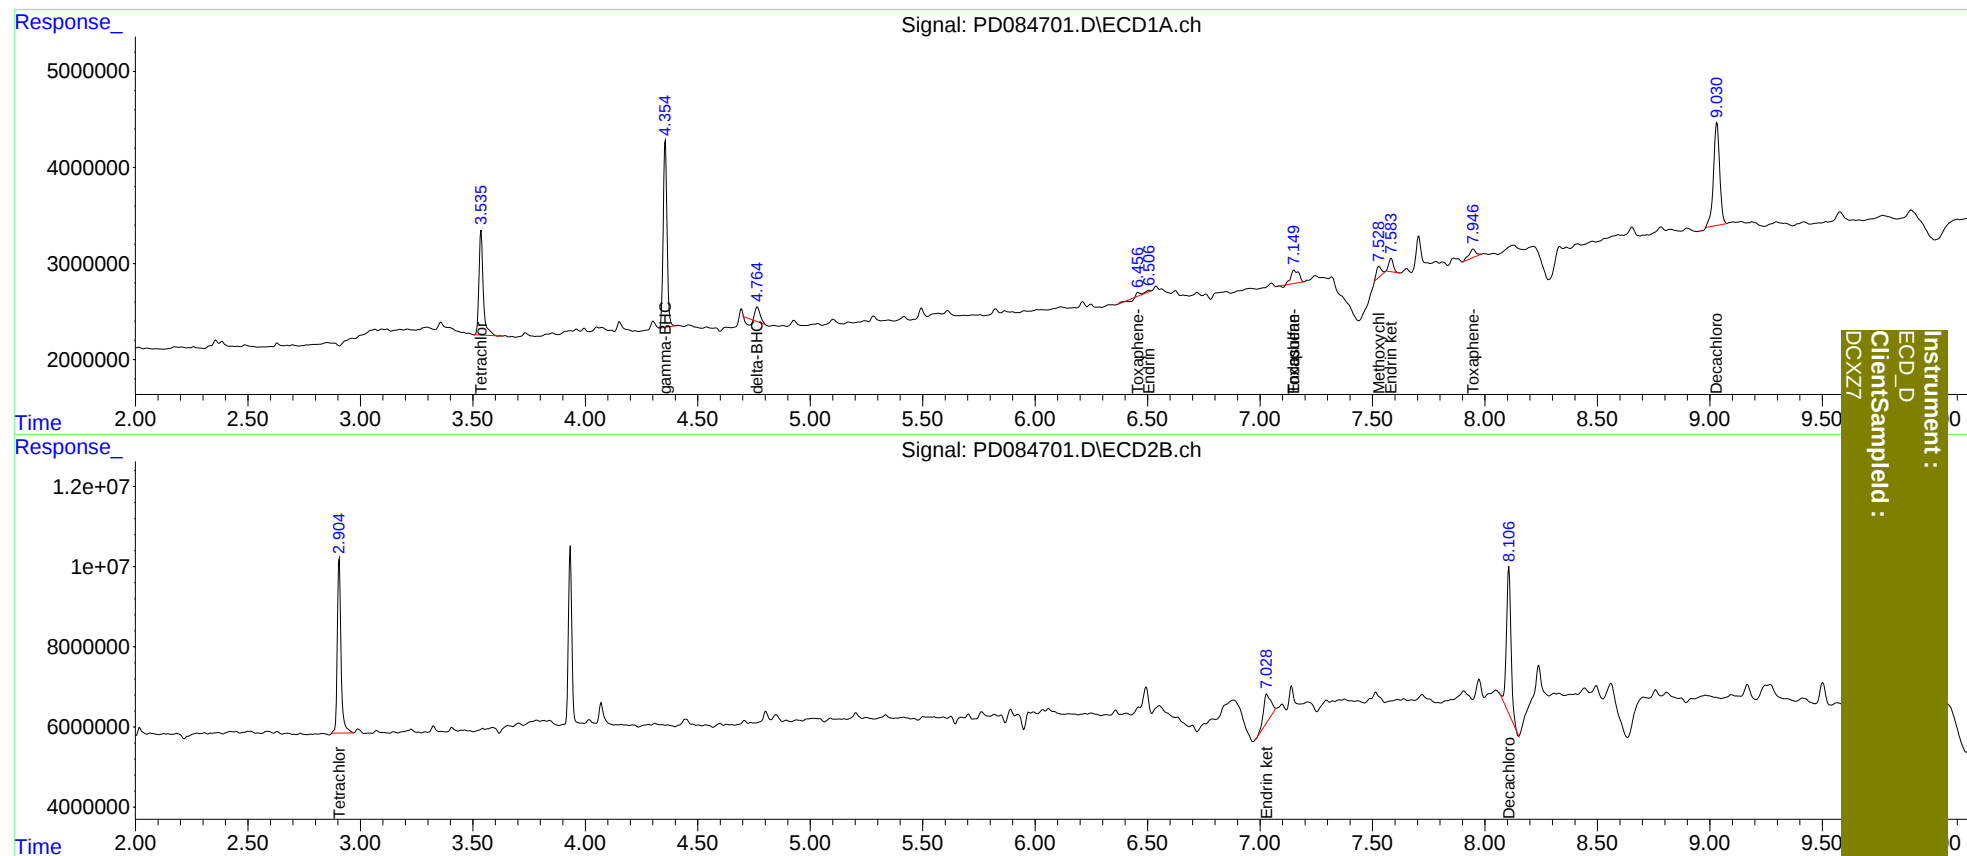

The printer must be in Portrait mode.

Instrument :
ECD_D
ClientSampleId :
DCXZ7