

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082724\
 Data File : PD084705.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2024 18:36
 Operator : AR\AJ
 Sample : P3626-22
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCYE4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 05:40:04 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.906	11530034	34402637	11.400	9.722
27)	SA Decachlor...	9.031	8.107	11843010	40388610	9.068	11.615 #
Target Compounds							
3)	MA gamma-BHC...	4.302	0.000	2634832	0	1.629	N.D. #
7)	B delta-BHC	4.766	0.000	2865890	0	1.747	N.D. #
12)	B 4,4'-DDE	6.211f	0.000	1392694	0	1.116	N.D. #
19)	B Endosulfa...	7.171f	6.532	986061	33633371	0.856	9.417 #
20)	A Methoxychlor	7.412f	0.000	1289055	0	2.475	N.D. #
23)	Toxaphene-2	6.456f	0.000	1137122	0	77.311	N.D. #
25)	Toxaphene-4	7.171f	0.000	986061	0	38.322	N.D. #
26)	Toxaphene-5	7.886	7.351	4163630	23355690	221.009	567.792 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082724\
Data File : PD084705.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2024 18:36
Operator : AR\AJ
Sample : P3626-22
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 05:40:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

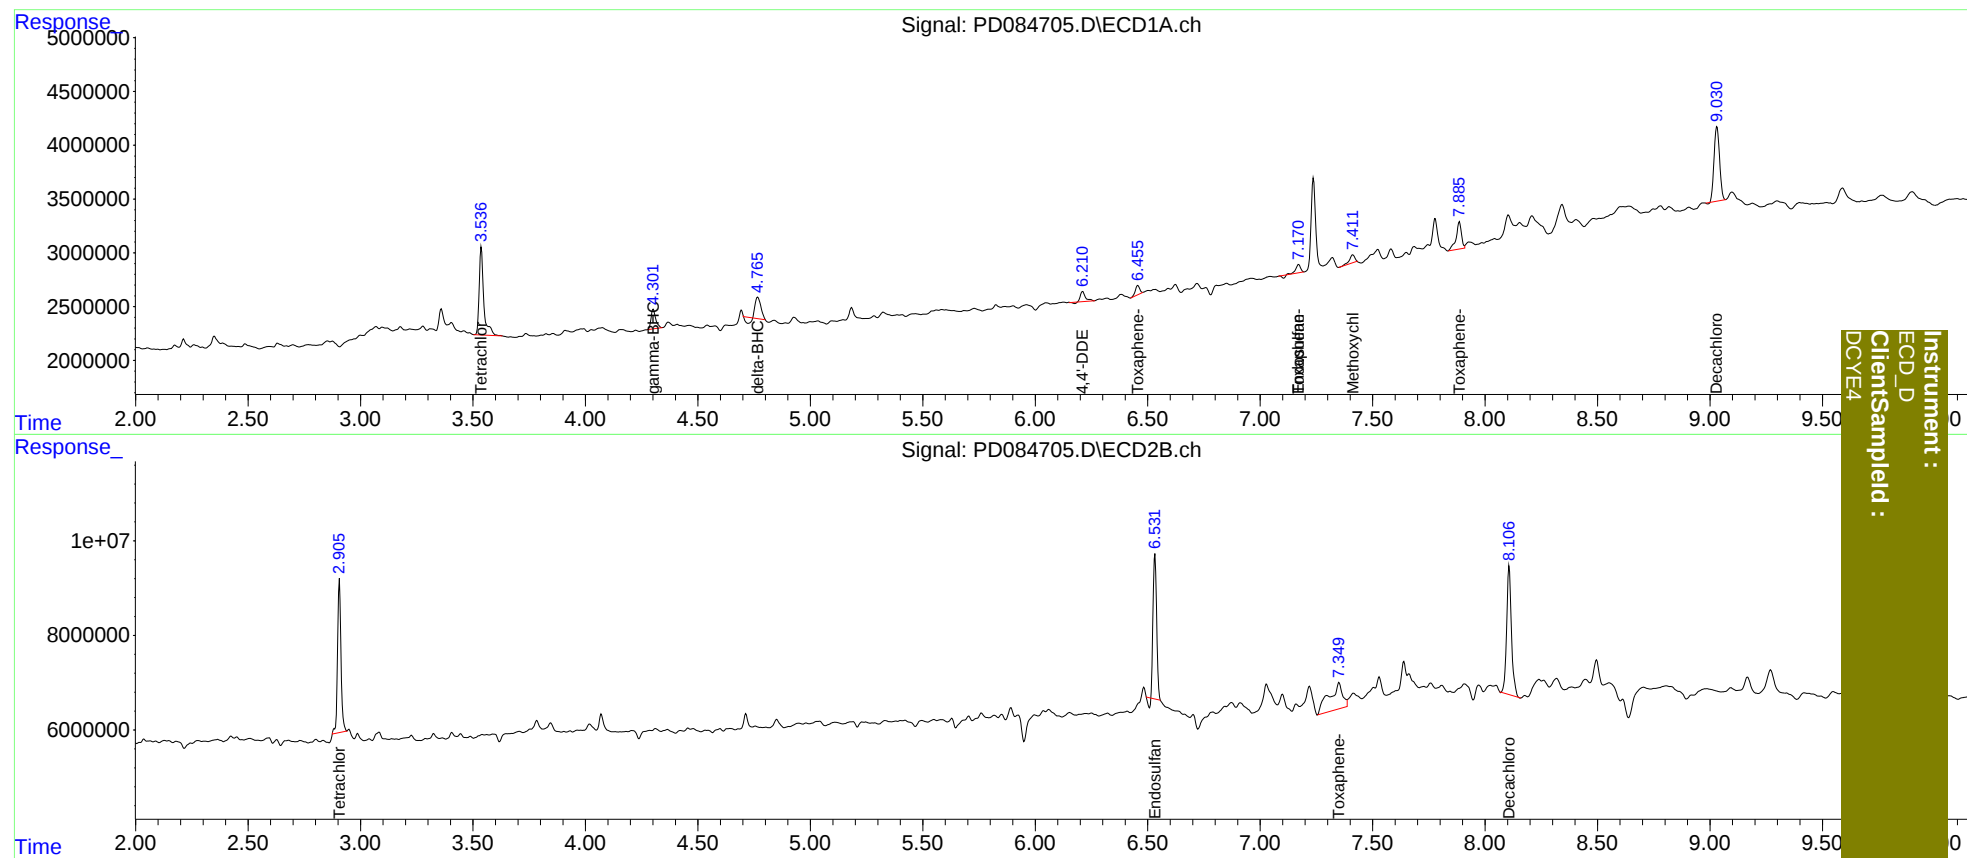

The printer must be in Portrait mode.

Instrument :
ECD_D
ClientSampleId :
DCYE4