

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082724\
 Data File : PD084709.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2024 19:43
 Operator : AR\AJ
 Sample : PB162899BS
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS899

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 05:40:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.906	20268403	69987425	20.040	19.777
27)	SA Decachlor...	9.031	8.107	33814683	87307140	25.891	25.108
Target Compounds							
2)	A alpha-BHC	3.982	3.417	7561216	24791707	4.447	4.890
3)	MA gamma-BHC...	4.311	3.752	7667259	25858777	4.739	5.336
4)	MA Heptachlor	4.909	4.107	8044899	22219763	5.229	5.220
5)	MB Aldrin	5.250	4.394	7787974	22506904	4.869	5.068
6)	B beta-BHC	4.494	4.045	3405907	10948033	4.689	5.050
7)	B delta-BHC	4.741	4.283	6909239	21355663	4.213	4.302
8)	B Heptachlo...	5.669	4.898	7689642	22783207	5.156	5.379
9)	A Endosulfan I	6.052	5.274	3735158	19497915	2.715	5.086 #
10)	B trans-Chl...	5.923	5.152	7277842	22260832	5.160	5.412
11)	B cis-Chlor...	6.005	5.217	7018904	23138947	4.747	5.515
12)	B 4,4'-DDE	6.173	5.402	12554443	41957285	10.064	10.696
13)	MA Dieldrin	6.324	5.541	14362264	46331250	9.736	10.784
14)	MA Endrin	6.550	5.818	11208012	42263683	9.933	11.415
15)	B Endosulfa...	6.761	6.110	13215229	42056109	10.011	11.343
16)	A 4,4'-DDD	6.680	5.958	10447733	40230922	10.582	11.855
17)	MA 4,4'-DDT	6.996	6.213	7860743	31559921	8.782	9.866
18)	B Endrin al...	6.889	6.289	10387162	32732093	11.502	11.464
19)	B Endosulfa...	7.123	6.513	11913050	38918263	10.341	10.897
20)	A Methoxychlor	7.467	6.786	25675226	88574589	49.289	53.543
21)	B Endrin ke...	7.603	7.023	13595286	53587116	11.120	12.170
22)	Toxaphene-1	0.000	5.152	0	22260832	N.D.	878.010
23)	Toxaphene-2	0.000	5.541f	0	46331250	N.D.	1874.485
24)	Toxaphene-3	6.996f	5.818f	7860743	42263683	229.433	1791.110 #
25)	Toxaphene-4	7.123	0.000	11913050	0	462.979	N.D. #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082724\
Data File : PD084709.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2024 19:43
Operator : AR\AJ
Sample : PB162899BS
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 05:40:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

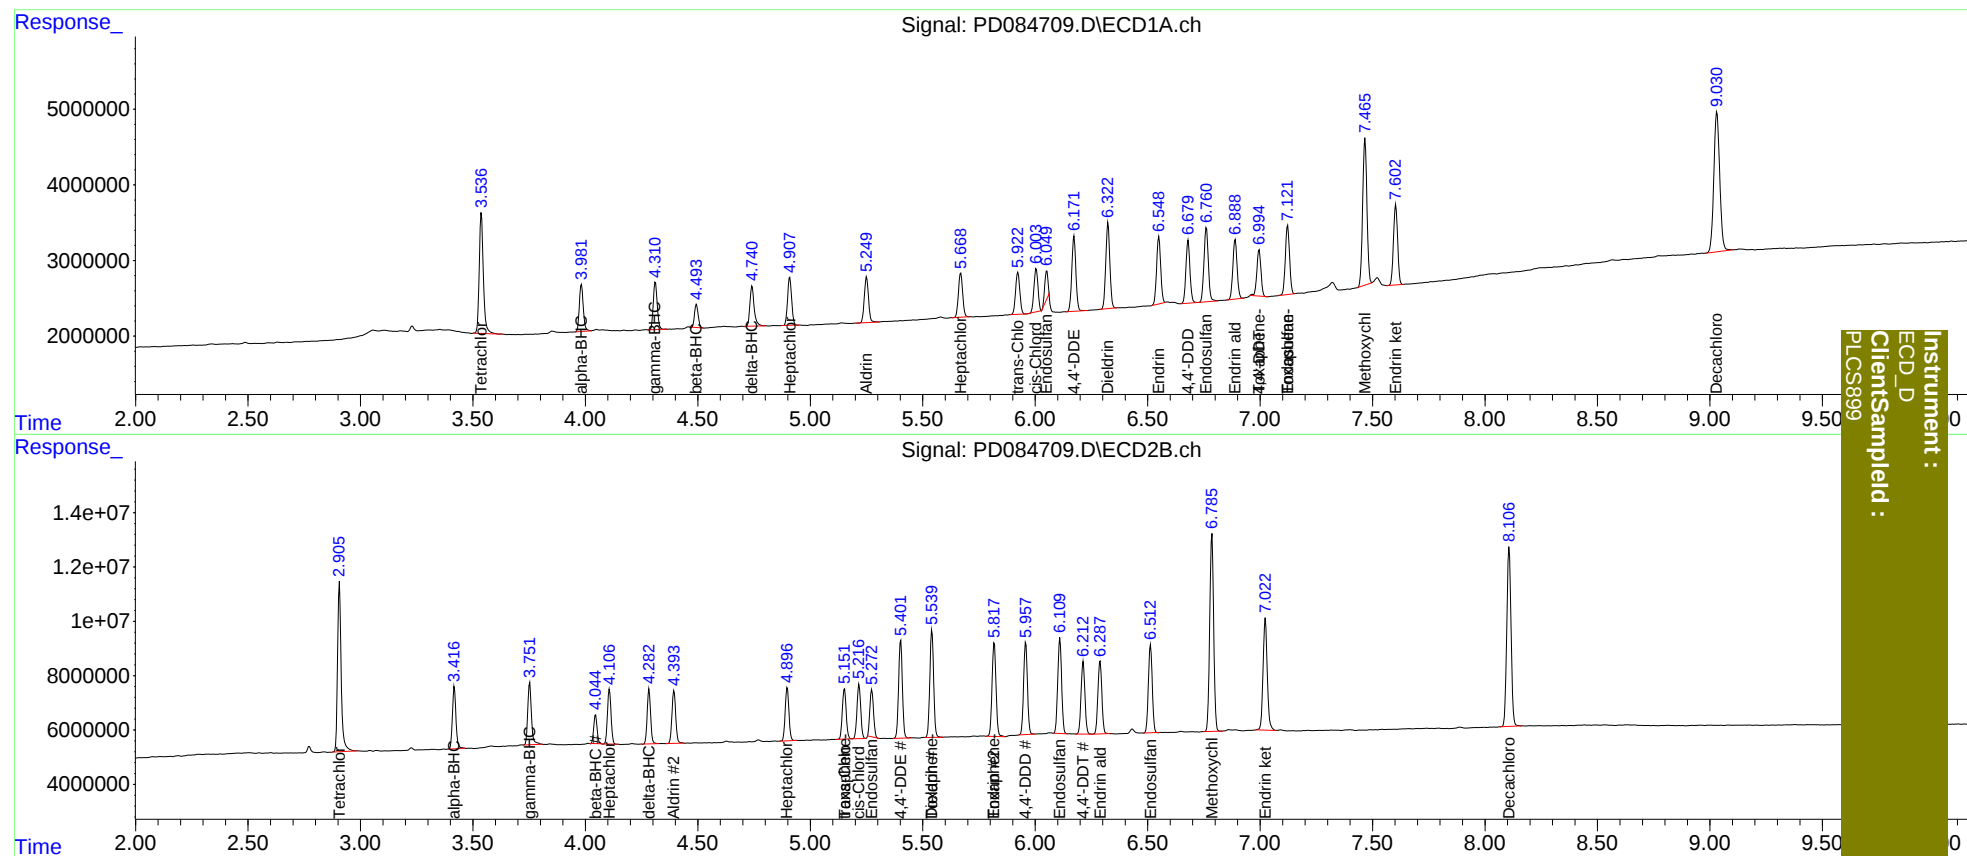

The printer must be in Portrait mode.

Instrument :
ECD_D
ClientSampleId :
PLCS899