

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082724\
 Data File : PD084710.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2024 19:56
 Operator : AR\AJ
 Sample : P3673-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCXY7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 05:41:10 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.906	6480345	28070978	6.407	7.932
27)	SA Decachlor...	9.031	8.107	6603301	41752852	5.056	12.008 #
Target Compounds							
7)	B delta-BHC	4.695f	0.000	1604019	0	0.978	N.D. #
18)	B Endrin al...	6.839f	0.000	3867557	0	4.283	N.D. #
19)	B Endosulfa...	7.171f	0.000	1389947	0	1.207	N.D. #
21)	B Endrin ke...	7.585	0.000	1938625	0	1.586	N.D. #
23)	Toxaphene-2	6.460f	0.000	1532818	0	104.214	N.D. #
25)	Toxaphene-4	7.171f	0.000	1389947	0	54.018	N.D. #
26)	Toxaphene-5	7.890	0.000	4859044	0	257.922	N.D. #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082724\
Data File : PD084710.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2024 19:56
Operator : AR\AJ
Sample : P3673-01
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 05:41:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

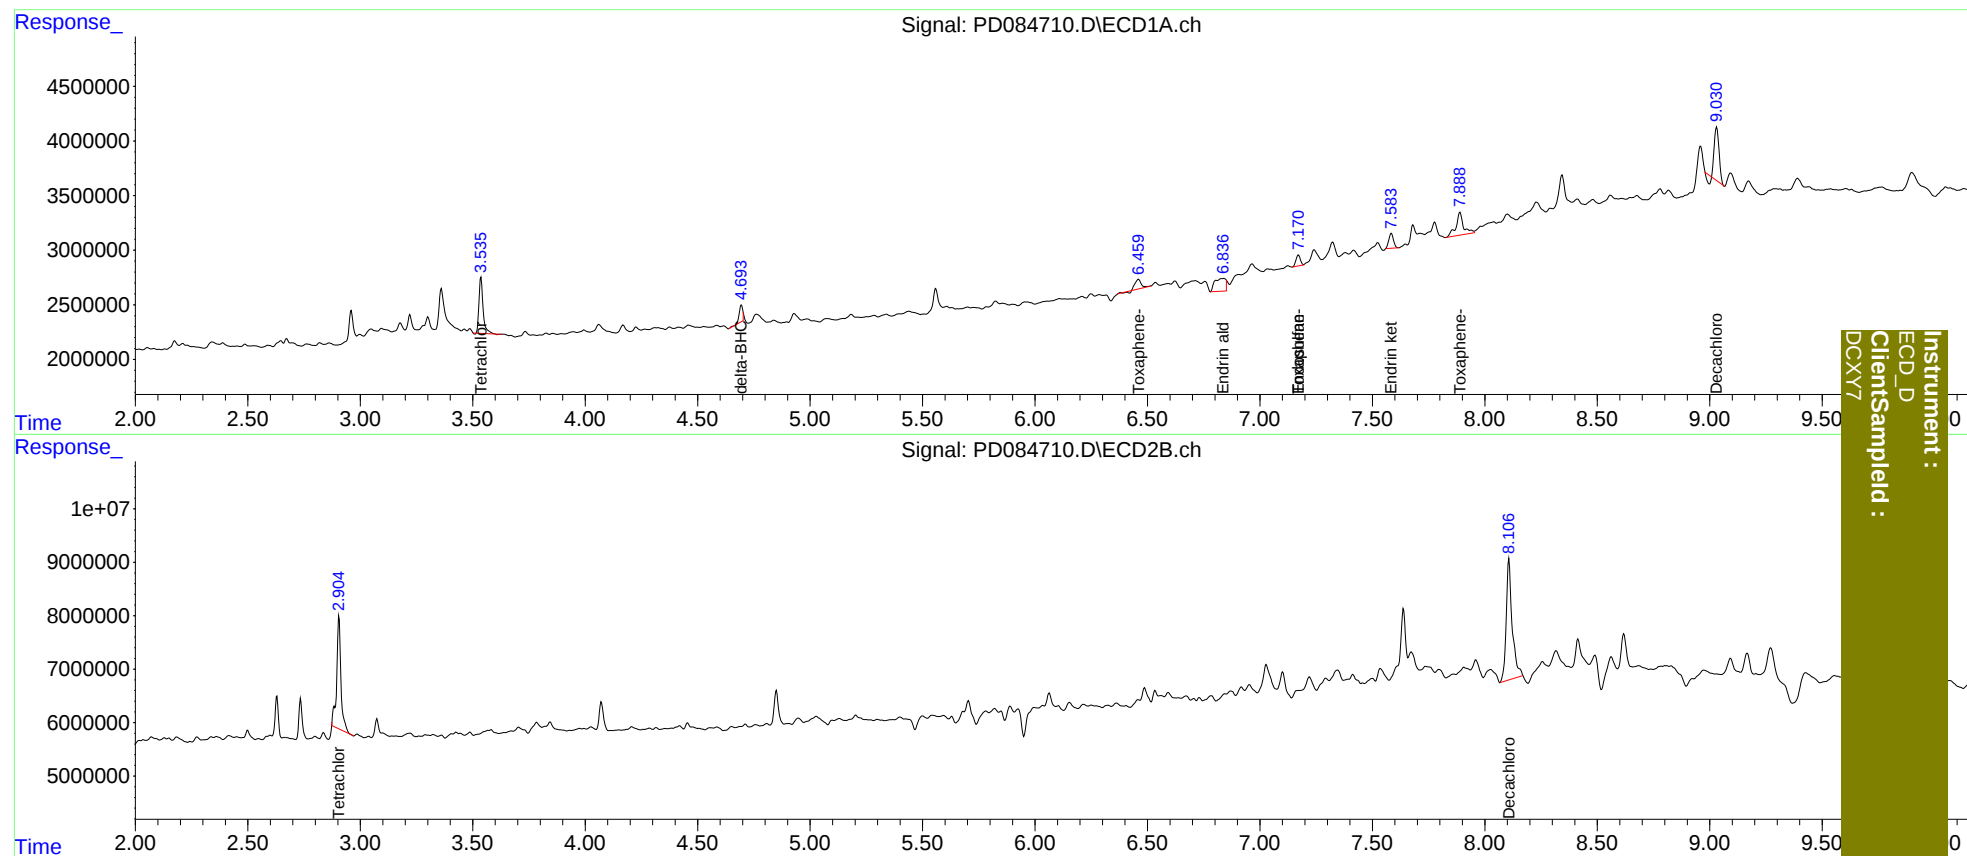

The printer must be in Portrait mode.

Instrument :
ECD_D
ClientSampleId :
DCXY7