

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082724\
 Data File : PD084729.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Aug 2024 00:37
 Operator : AR\AJ
 Sample : P3673-21MS
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCXZ4MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 05:44:54 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.907	13332911	47034518	13.183	13.291
27)	SA Decachlor...	9.031	8.107	15852969	43218989	12.138	12.429
Target Compounds							
2)	A alpha-BHC	3.983	3.418	104.4E6	290.6E6	61.417	57.320
3)	MA gamma-BHC...	4.312	3.752	100.5E6	277.7E6	62.105	57.315
4)	MA Heptachlor	4.909	4.107	96726171	246.8E6	62.866	57.979
5)	MB Aldrin	5.250	4.394	95600123	246.1E6	59.774	55.413
6)	B beta-BHC	4.494	4.045	39685326	115.4E6	54.635	53.226
7)	B delta-BHC	4.742	4.283	100.5E6	281.4E6	61.306	56.687
8)	B Heptachlo...	5.669	4.897	84649152	228.3E6	56.756	53.901
9)	A Endosulfan I	6.051	5.274	42751362	179.6E6	31.074	46.851 #
10)	B trans-Chl...	5.923	5.152	83147822	229.3E6	58.954	55.741
11)	B cis-Chlor...	6.004	5.216	79510919	230.3E6	53.776	54.891
12)	B 4,4'-DDE	6.173	5.402	160.4E6	451.5E6	128.564	115.109
13)	MA Dieldrin	6.324	5.540	177.8E6	479.9E6	120.516	111.704
14)	MA Endrin	6.550	5.818	154.0E6	447.0E6	136.488	120.747
15)	B Endosulfa...	6.761	6.109	146.5E6	409.0E6	111.006	110.298
16)	A 4,4'-DDD	6.680	5.958	129.9E6	394.3E6	131.598	116.199
17)	MA 4,4'-DDT	6.996	6.213	105.2E6	350.9E6	117.549	109.708
18)	B Endrin al...	6.889	6.288	107.9E6	304.1E6	119.453	106.502
19)	B Endosulfa...	7.123	6.513	139.3E6	395.3E6	120.947	110.686
20)	A Methoxychlor	7.466	6.786	317.3E6	865.8E6	609.026	523.357
21)	B Endrin ke...	7.602	7.023	154.6E6	464.2E6	126.412	105.432
22)	Toxaphene-1	0.000	5.152	0	229.3E6	N.D.	9042.940
23)	Toxaphene-2	6.454f	5.540f	14603171	479.9E6	992.847	19415.784 #
24)	Toxaphene-3	6.996f	5.893	105.2E6	18019131	3071.116	763.640 #
25)	Toxaphene-4	7.123	0.000	139.3E6	0	5414.896	N.D. #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082724\
Data File : PD084729.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Aug 2024 00:37
Operator : AR\AJ
Sample : P3673-21MS
Misc :
ALS Vial : 47 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 05:44:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

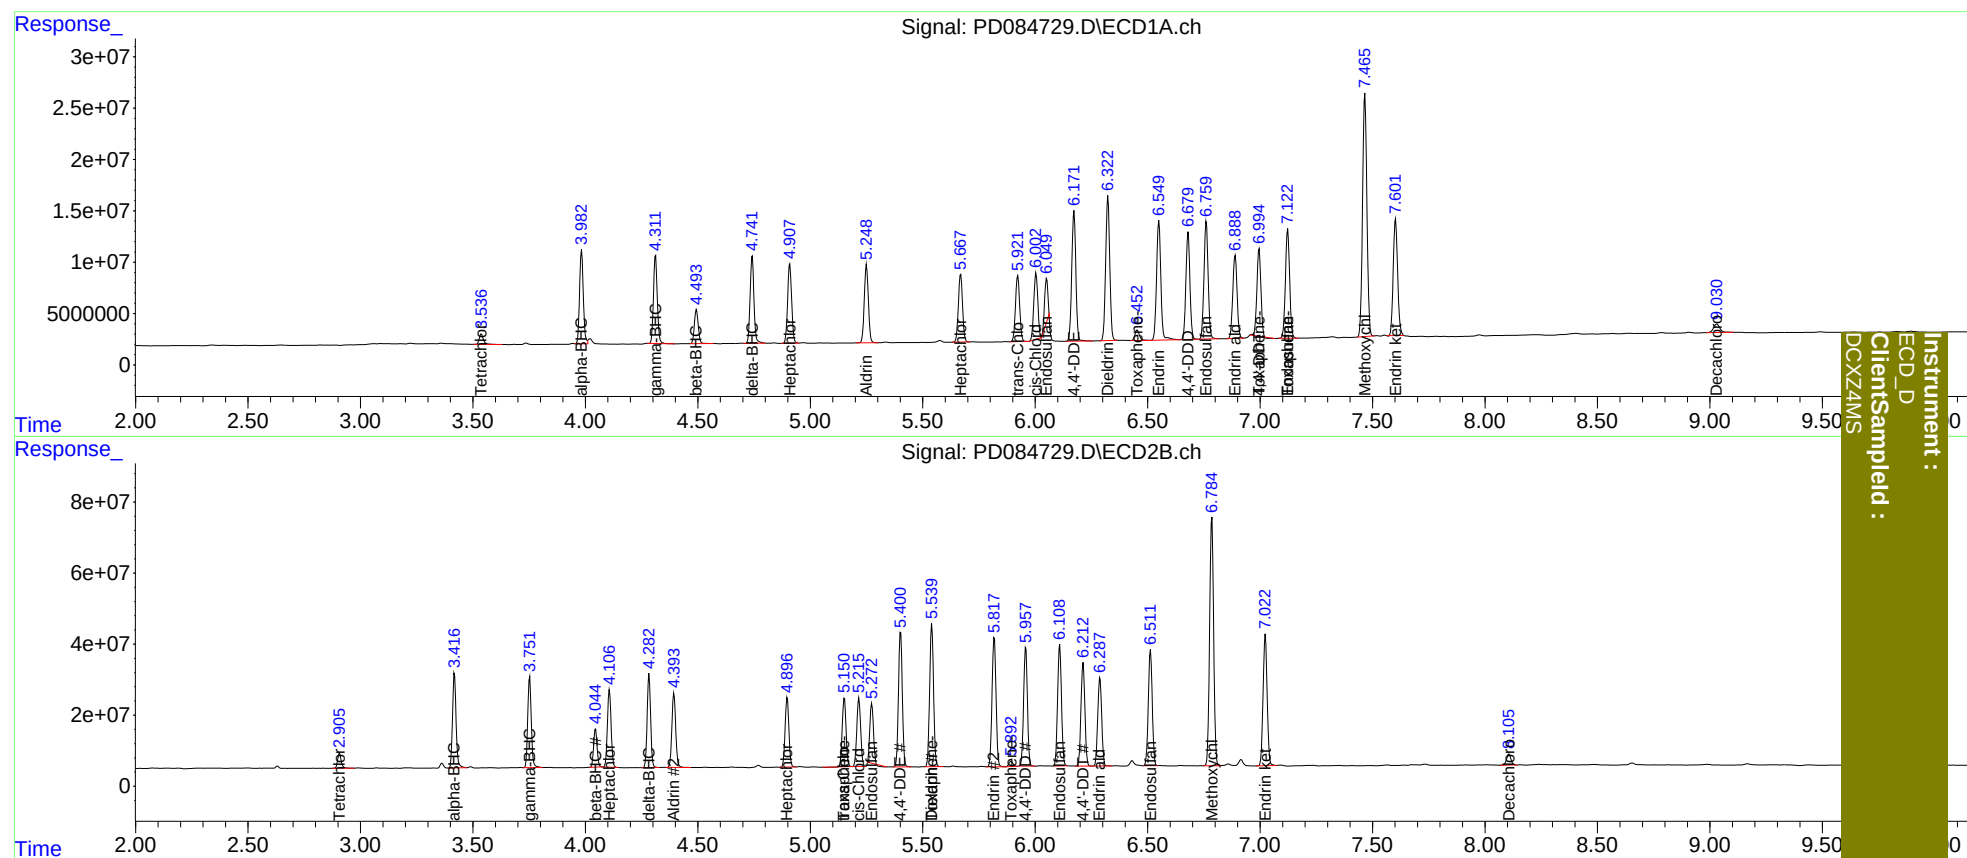

The printer must be in Portrait mode.

Instrument :
ECD_D
ClientSampleId :
DCXZ4MS