

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082921\
 Data File : PD065395.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2021 10:34
 Operator : AR\AJ
 Sample : RESC12
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC009

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 14:45:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082921CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 27 14:43:58 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	22032526	160.0E6	19.489	19.751
2)	SA Decachlor...	8.239	9.083	55904744	205.8E6	38.698	39.787
Target Compounds							
2)	A alpha-BHC	3.935	4.408	14915816	112.0E6	9.688	10.255
3)	MA gamma-BHC...	4.218	4.695	16112930	108.1E6	9.848	10.281
4)	MA Heptachlor	4.516	5.198	14967236	105.4E6	10.210	10.471
5)	MB Aldrin	4.764	5.503	14801411	102.5E6	10.484	10.717
6)	B beta-BHC	4.466	4.870	8600339	52518870	11.657	10.940
7)	B delta-BHC	4.671	5.087	15229727	106.7E6	10.142	10.277
8)	B Heptachlo...	5.206	5.893	14065913	84853632	10.430	10.403
9)	A Endosulfan I	5.545	6.251	13017348	75137098	10.211	10.133
10)	B trans-Chl...	5.431	6.126	14259568	85842717	10.429	10.584
11)	B cis-Chlor...	5.490	6.198	14119026	82479295	10.405	10.405
12)	B 4,4'-DDE	5.653	6.356	24871705	155.2E6	19.926	20.966
13)	MA Dieldrin	5.788	6.508	26642217	156.2E6	19.908	20.419
14)	MA Endrin	6.046	6.728	24571560	132.5E6	20.177	20.920
15)	B Endosulfa...	6.318	6.941	26123740	137.2E6	20.740	21.157
16)	A 4,4'-DDD	6.168	6.850	21795585	123.0E6	19.859	20.441
17)	MA 4,4'-DDT	6.408	7.148	23618584	127.5E6	19.690	20.897
18)	B Endrin al...	6.487	7.065	21286384	110.2E6	21.232	21.544
19)	B Endosulfa...	6.698	7.287	26836515	132.7E6	20.969	21.340
20)	A Methoxychlor	6.954	7.607	67320510	311.1E6	102.964	106.609
21)	B Endrin ke...	7.192	7.761	33120329	153.8E6	21.315	21.652

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082921\
Data File : PD065395.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2021 10:34
Operator : AR\AJ
Sample : RESC12
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 14:45:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082921CLP.M
Quant Title : GC Extractables
QLast Update : Fri Aug 27 14:43:58 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

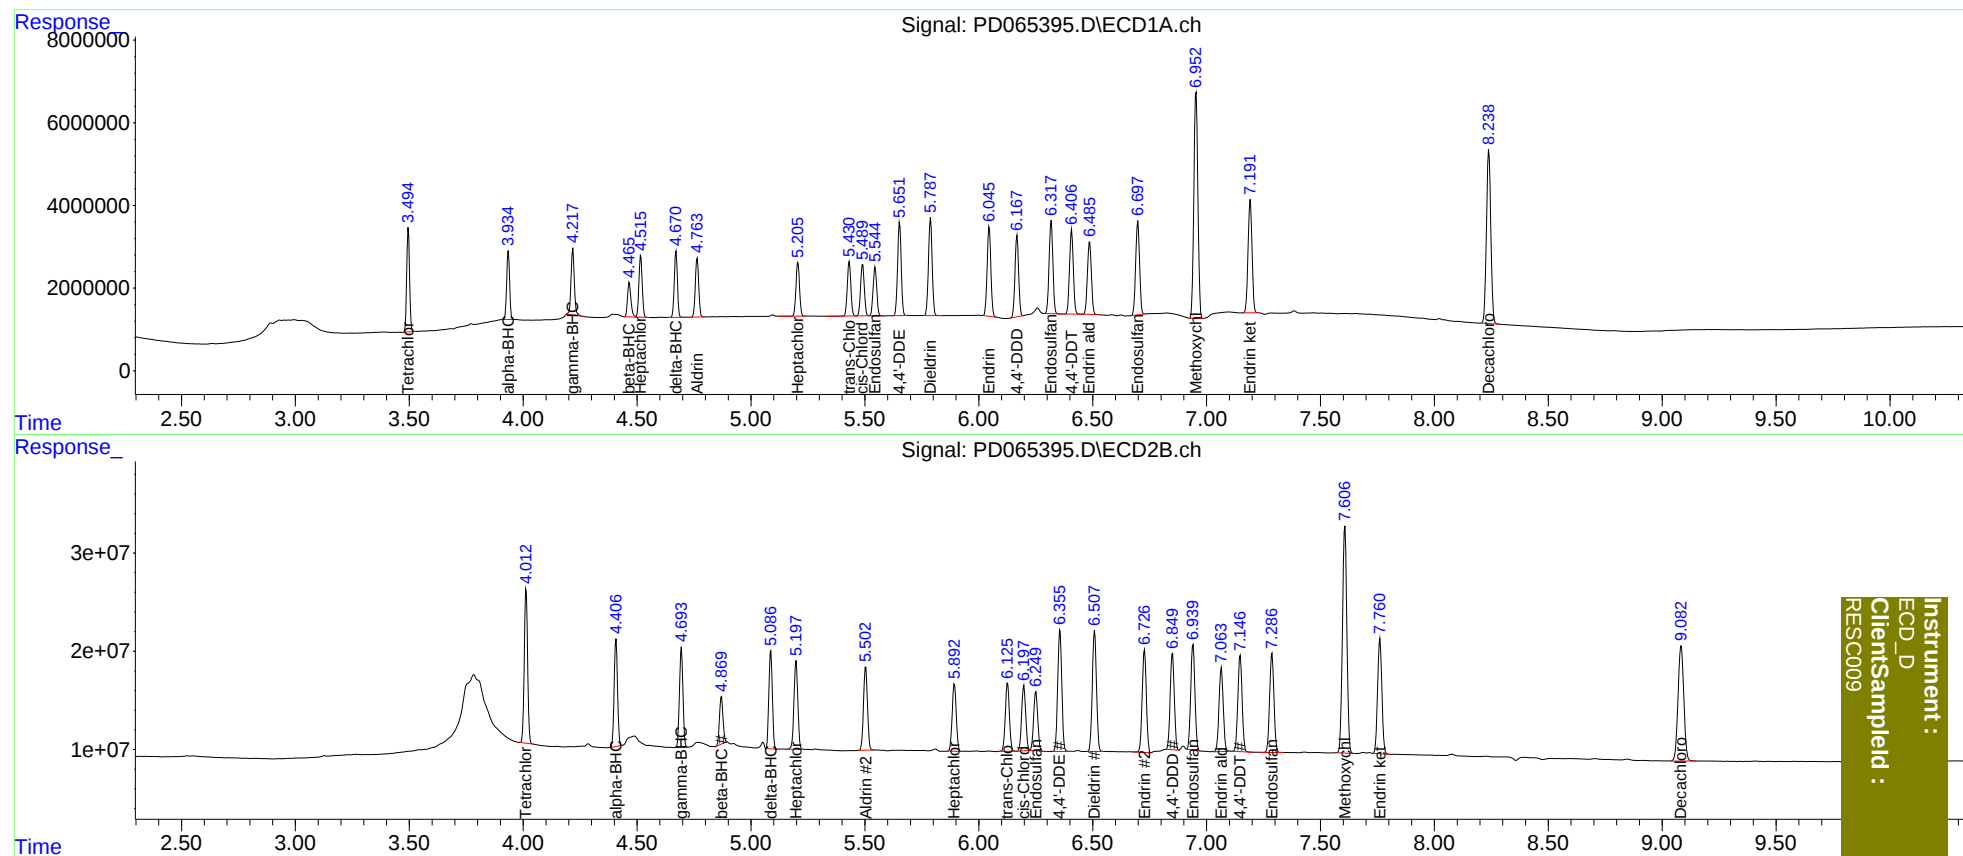

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082921\
Data File : PD065395.D
Acq On : 27 Aug 2021 10:34
Operator : AR\AJ
Sample : RESC12
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC009

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082921CLP.M
Title : GC Extractables
Last Update : Fri Aug 27 14:43:58 2021
Integrator: ChemStation

RT#1	RT#2	Resolution
3.496	3.935	100.00%
3.935	4.218	100.00%
4.218	4.466	100.00%
4.466	4.516	100.00%
4.516	4.671	100.00%
4.671	4.764	100.00%
4.764	5.206	100.00%
5.206	5.431	100.00%
5.431	5.490	100.00%
5.490	5.545	100.00%
5.545	5.653	100.00%
5.653	5.788	100.00%
5.788	6.046	100.00%
6.046	6.168	100.00%
6.168	6.318	100.00%
6.318	6.408	100.00%
6.408	6.487	100.00%
6.487	6.698	100.00%
6.698	6.954	100.00%
6.954	7.192	100.00%
7.192	8.239	100.00%

Signal #2

4.013	4.408	100.00%
4.408	4.695	100.00%
4.695	4.870	100.00%
4.870	5.087	100.00%
5.087	5.198	100.00%
5.198	5.503	100.00%
5.503	5.893	100.00%
5.893	6.126	100.00%
6.126	6.198	100.00%
6.198	6.251	100.00%
6.251	6.356	100.00%
6.356	6.509	100.00%
6.509	6.728	100.00%
6.728	6.850	100.00%
6.850	6.941	100.00%
6.941	7.065	100.00%
7.065	7.148	100.00%
7.148	7.287	100.00%
7.287	7.607	100.00%
7.607	7.761	100.00%
7.761	9.083	100.00%