

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082923\
 Data File : PD077405.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2023 18:15
 Operator : AR\AJ
 Sample : 04148-02MS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH8S3MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 22:00:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:53:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.762	46560901	25194106	21.208	20.224
27)	SA Decachlor...	9.083	7.900	97265189	48696481	38.224	39.066
Target Compounds							
2)	A alpha-BHC	4.000	3.263	227.7E6	114.6E6	63.019	62.359
3)	MA gamma-BHC...	4.333	3.593	205.1E6	104.1E6	60.095	60.363
4)	MA Heptachlor	4.923	3.932	185.7E6	100.4E6	53.081	58.288
5)	MB Aldrin	5.266	4.212	206.9E6	117.0E6	59.712	67.633
6)	B beta-BHC	4.530	3.890	82630862	43055115	53.245	52.740
7)	B delta-BHC	4.778	4.120	204.9E6	107.6E6	61.822	61.943
8)	B Heptachlo...	5.694	4.713	180.2E6	91873040	56.462	56.160
9)	A Endosulfan I	6.081	5.083	174.0E6	87493782	61.550	62.099
10)	B trans-Chl...	5.951	4.964	182.7E6	93370286	59.164	60.456
11)	B cis-Chlor...	6.030	5.027	185.3E6	94153142	57.863	58.462
12)	B 4,4'-DDE	6.203	5.216	363.7E6	179.7E6	126.972	132.046
13)	MA Dieldrin	6.357	5.348	395.0E6	199.9E6	126.710	126.051
14)	MA Endrin	6.587	5.624	325.9E6	174.6E6	128.191	125.806
15)	B Endosulfa...	6.807	5.918	324.0E6	167.5E6	114.646	125.164
16)	A 4,4'-DDD	6.721	5.771	289.5E6	141.9E6	133.219	142.709
17)	MA 4,4'-DDT	7.036	6.022	301.6E6	144.2E6	136.705	139.272
18)	B Endrin al...	6.937	6.098	235.7E6	121.8E6	109.516	112.080
19)	B Endosulfa...	7.172	6.321	296.4E6	153.1E6	119.107	122.310
20)	A Methoxychlor	7.511	6.598	731.7E6	340.3E6	568.755	603.384
21)	B Endrin ke...	7.659	6.827	344.9E6	185.1E6	122.541	125.735

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082923\
Data File : PD077405.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2023 18:15
Operator : AR\AJ
Sample : 04148-02MS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 22:00:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 01:53:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

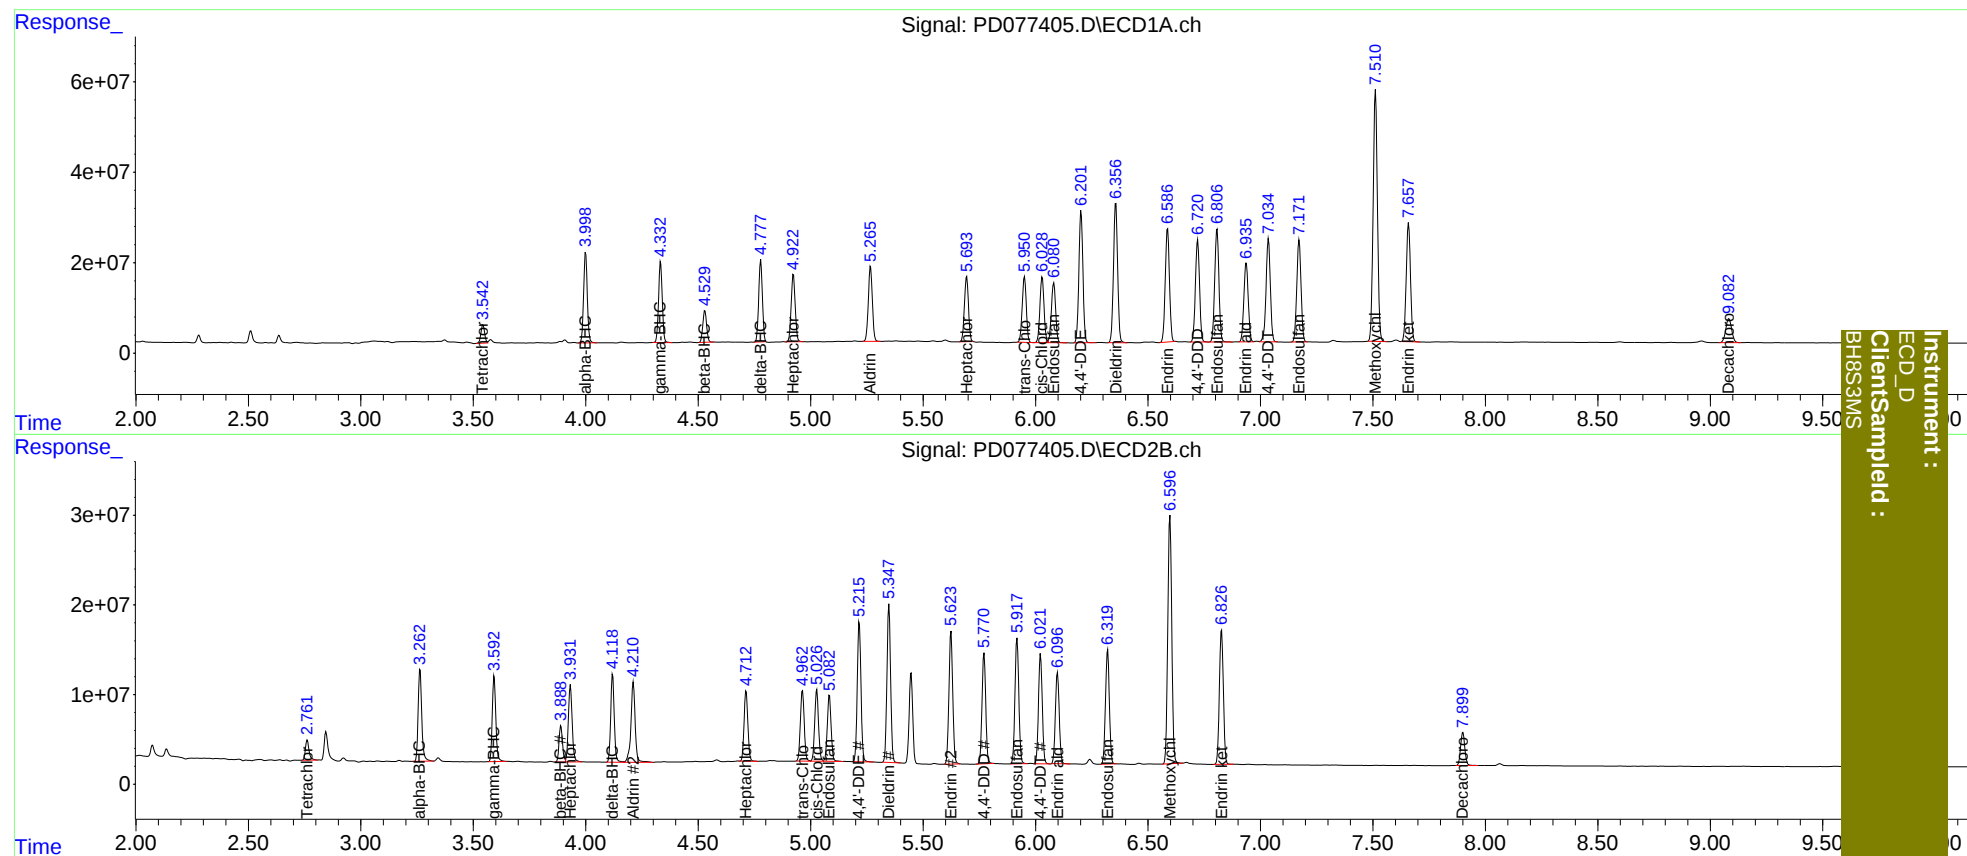

Instrument :
ECD_D
ClientSampled :
BH8S3MS