

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082923\
 Data File : PD077406.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2023 18:28
 Operator : AR\AJ
 Sample : 04148-03MSD
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH8S3MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 22:00:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:53:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.762	46574021	25401312	21.214	20.390
2)	SA Decachlor...	9.082	7.901	97707018	49239918	38.398	39.502
Target Compounds							
2)	A alpha-BHC	3.999	3.263	228.4E6	115.5E6	63.228	62.818
3)	MA gamma-BHC...	4.332	3.593	205.8E6	105.0E6	60.287	60.868
4)	MA Heptachlor	4.923	3.932	187.9E6	101.6E6	53.710	58.972
5)	MB Aldrin	5.266	4.211	208.4E6	119.5E6	60.157	69.028
6)	B beta-BHC	4.529	3.889	83117636	43366970	53.559	53.122
7)	B delta-BHC	4.777	4.119	206.0E6	108.6E6	62.138	62.519
8)	B Heptachlo...	5.693	4.713	181.8E6	92876449	56.959	56.774
9)	A Endosulfan I	6.080	5.084	174.0E6	88498286	61.548	62.812
10)	B trans-Chl...	5.950	4.964	183.9E6	94156238	59.540	60.965
11)	B cis-Chlor...	6.029	5.028	185.8E6	95067749	58.044	59.030
12)	B 4,4'-DDE	6.202	5.217	364.6E6	181.1E6	127.286	133.066
13)	MA Dieldrin	6.356	5.348	394.5E6	201.3E6	126.576	126.898
14)	MA Endrin	6.587	5.624	326.5E6	176.3E6	128.412	127.041
15)	B Endosulfa...	6.806	5.918	324.8E6	169.2E6	114.918	126.428
16)	A 4,4'-DDD	6.720	5.771	290.6E6	143.1E6	133.723	143.858
17)	MA 4,4'-DDT	7.036	6.022	305.6E6	146.4E6	138.506	141.374
18)	B Endrin al...	6.937	6.098	236.8E6	123.0E6	109.990	113.227
19)	B Endosulfa...	7.171	6.320	297.6E6	155.0E6	119.568	123.799
20)	A Methoxychlor	7.511	6.598	741.4E6	347.9E6	576.293	616.782
21)	B Endrin ke...	7.658	6.826	346.7E6	187.4E6	123.179	127.290

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082923\
Data File : PD077406.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2023 18:28
Operator : AR\AJ
Sample : 04148-03MSD
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 22:00:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 01:53:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

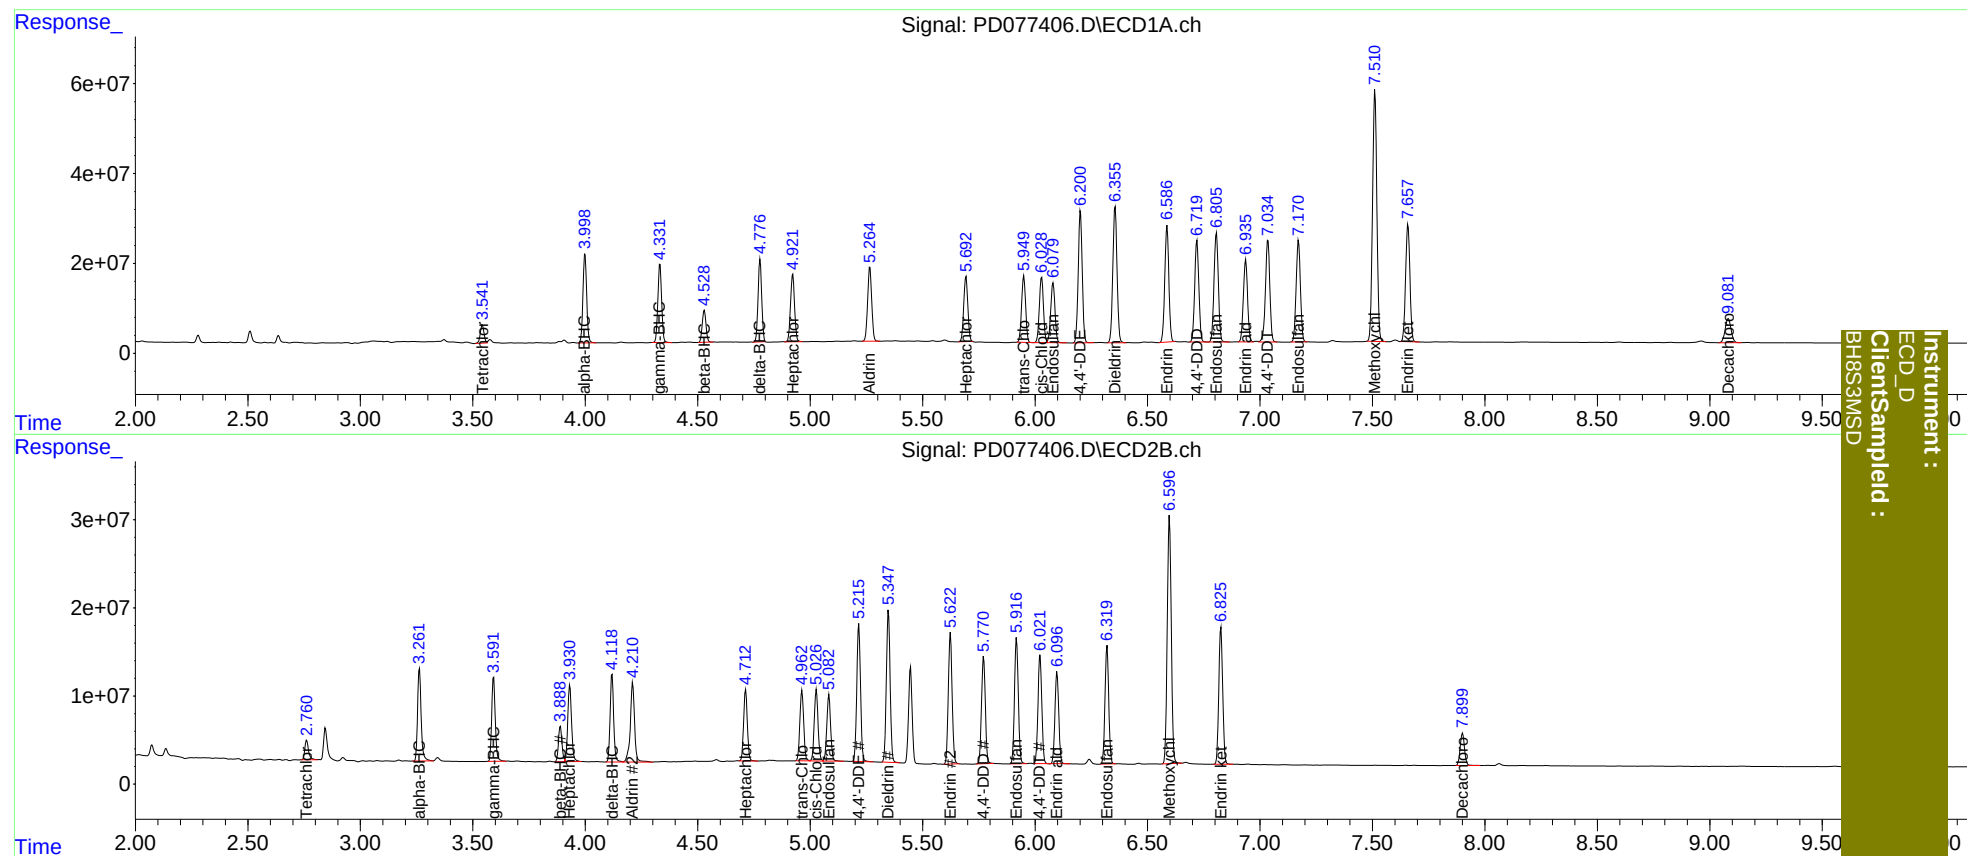

Instrument :
ECD_D
ClientSampled :
BH83MSD