

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082924\
 Data File : PD084770.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2024 11:31
 Operator : AR\AJ
 Sample : P3673-19
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCYI9

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 02:02:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.906	10583564	34612623	10.464	9.781
2)	SA Decachlor...	9.033	8.107	11060328	34718970	8.469	9.985
Target Compounds							
2)	A alpha-BHC	4.023f	0.000	9010950	0	5.300	N.D. #
7)	B delta-BHC	4.764	0.000	3194142	0	1.948	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD082924\
Data File : PD084770.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2024 11:31
Operator : AR\AJ
Sample : P3673-19
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 02:02:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

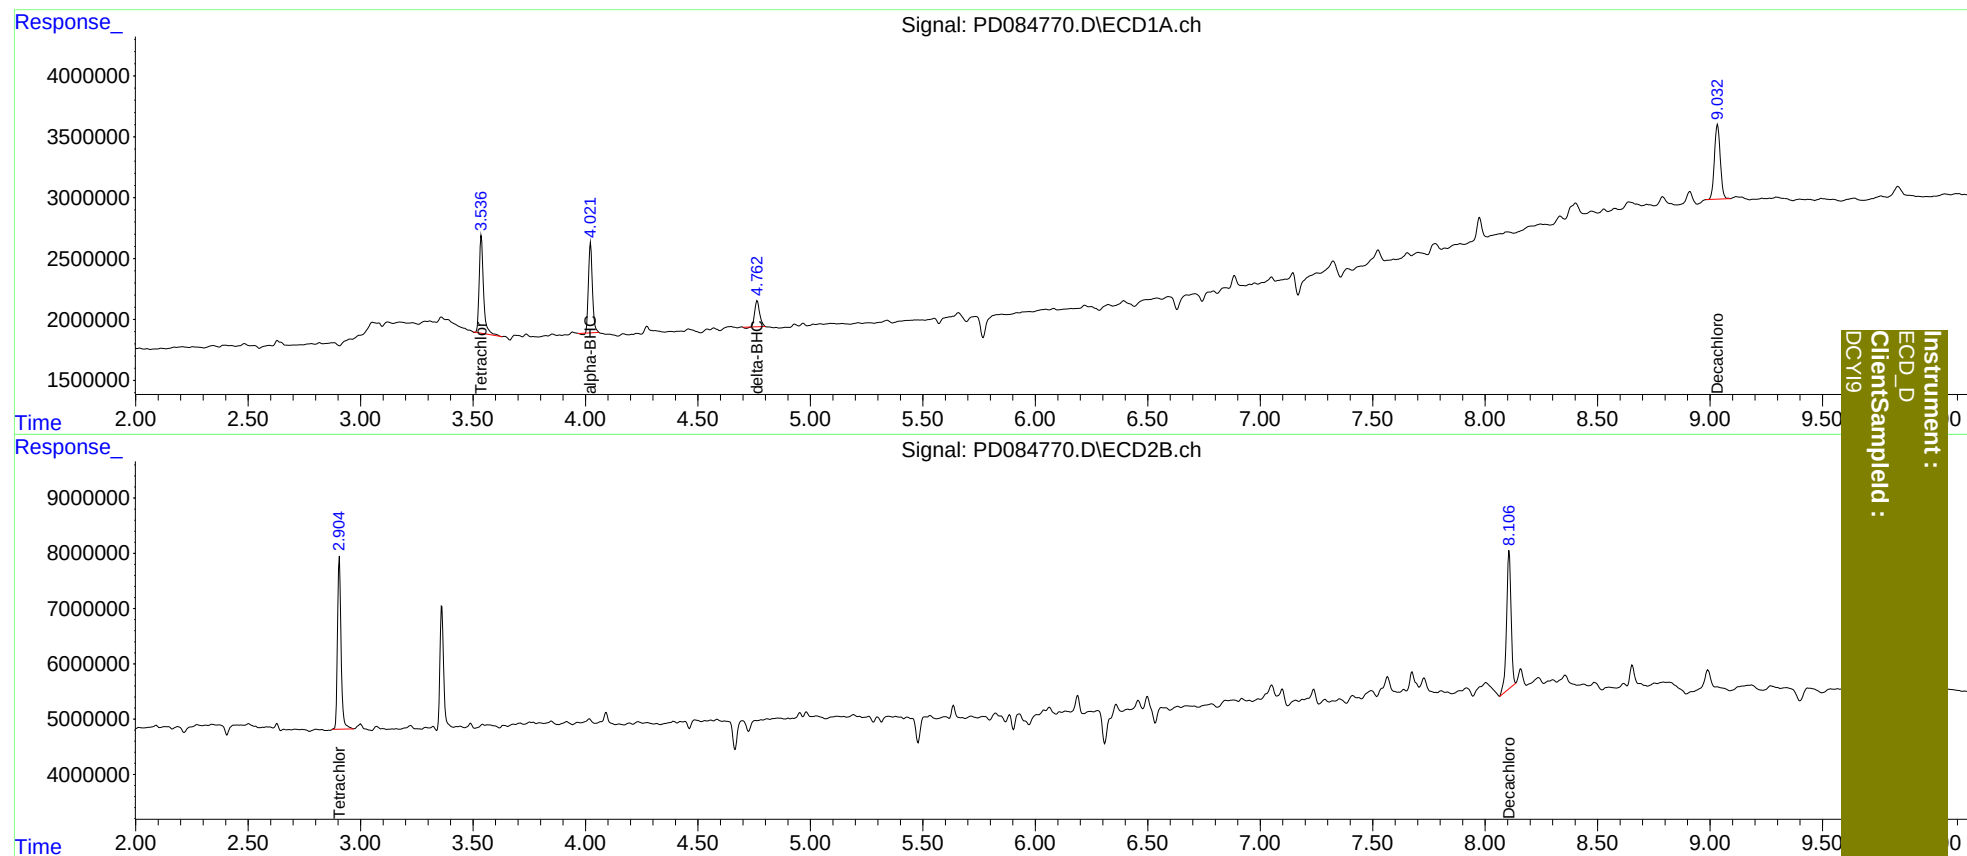


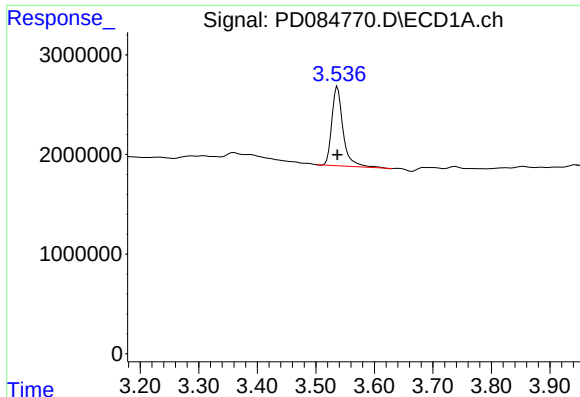

#1 Tetrachloro-m-xylene


R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 10583564
Conc: 10.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
DCYI9

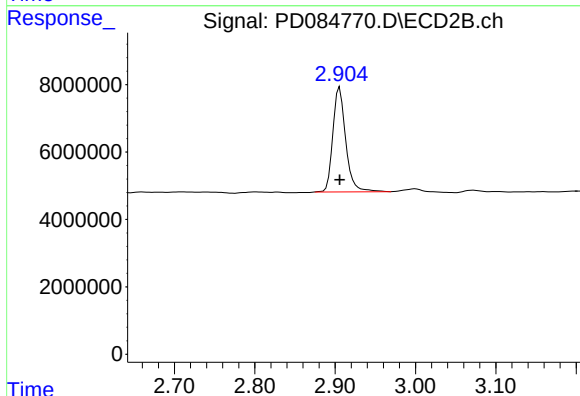


#1 Tetrachloro-m-xylene

R.T.: 2.906 min
Delta R.T.: 0.000 min
Response: 34612623
Conc: 9.78 ng/ml

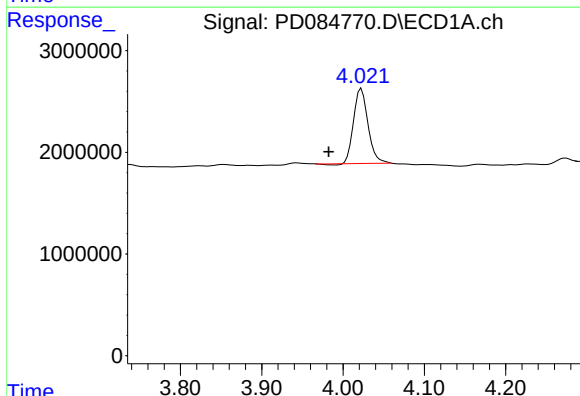


#2 alpha-BHC

R.T.: 4.023 min
Delta R.T.: 0.040 min
Response: 9010950
Conc: 5.30 ng/ml

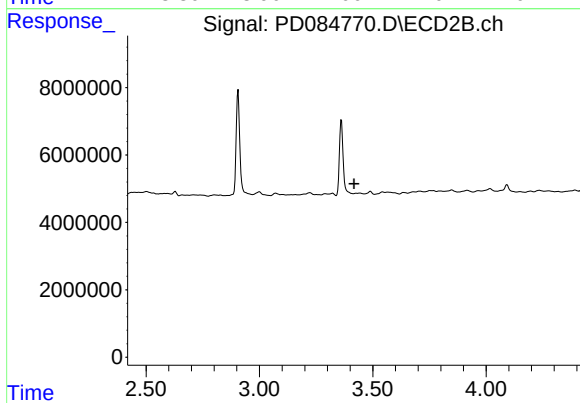

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 3.417 min
Response: 0
Conc: N.D.

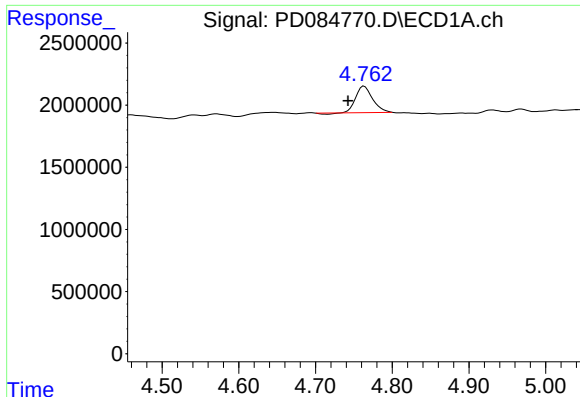

#7 delta-BHC


R.T.: 4.764 min
Delta R.T.: 0.021 min
Response: 3194142
Conc: 1.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
DCYI9

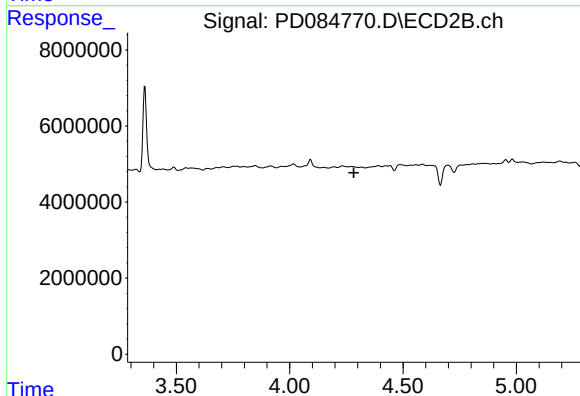


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.283 min
Response: 0
Conc: N.D.

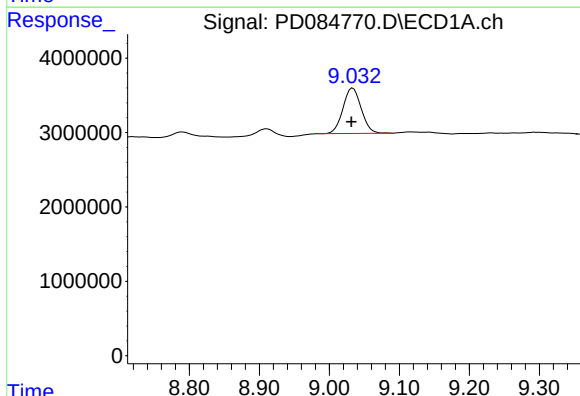

#27 Decachlorobiphenyl

R.T.: 9.033 min
Delta R.T.: 0.002 min
Response: 11060328
Conc: 8.47 ng/ml

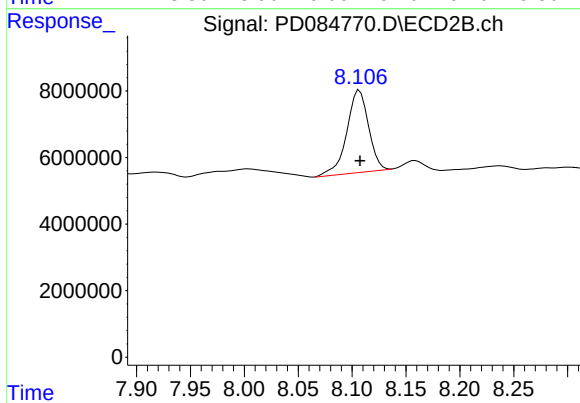

#27 Decachlorobiphenyl

R.T.: 8.107 min
Delta R.T.: 0.000 min
Response: 34718970
Conc: 9.98 ng/ml