

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083018\
 Data File : PD049067.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Aug 2018 18:39
 Operator : AJ\SJ
 Sample : PIBLK15
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK15

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 02:10:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081618CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 16 13:32:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.370	3.968	24910698	365.8E6	20.409	20.805
27)	SA Decachlor...	8.066	8.993	57995617	654.4E6	40.278	40.423
Target Compounds							
6)	B beta-BHC	0.000	4.766	0	6780284	N.D.	0.646
7)	B delta-BHC	0.000	5.048f	0	5394362	N.D.	0.237
9)	A Endosulfan I	0.000	6.193	0	4687230	N.D.	0.219
10)	B trans-Chl...	0.000	6.012f	0	4304696	N.D.	0.186
11)	B cis-Chlor...	0.000	6.193f	0	4687230	N.D.	0.204


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083018\
Data File : PD049067.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Aug 2018 18:39
Operator : AJ\SJ
Sample : PIBLK15
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK15

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 02:10:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081618CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 16 13:32:25 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

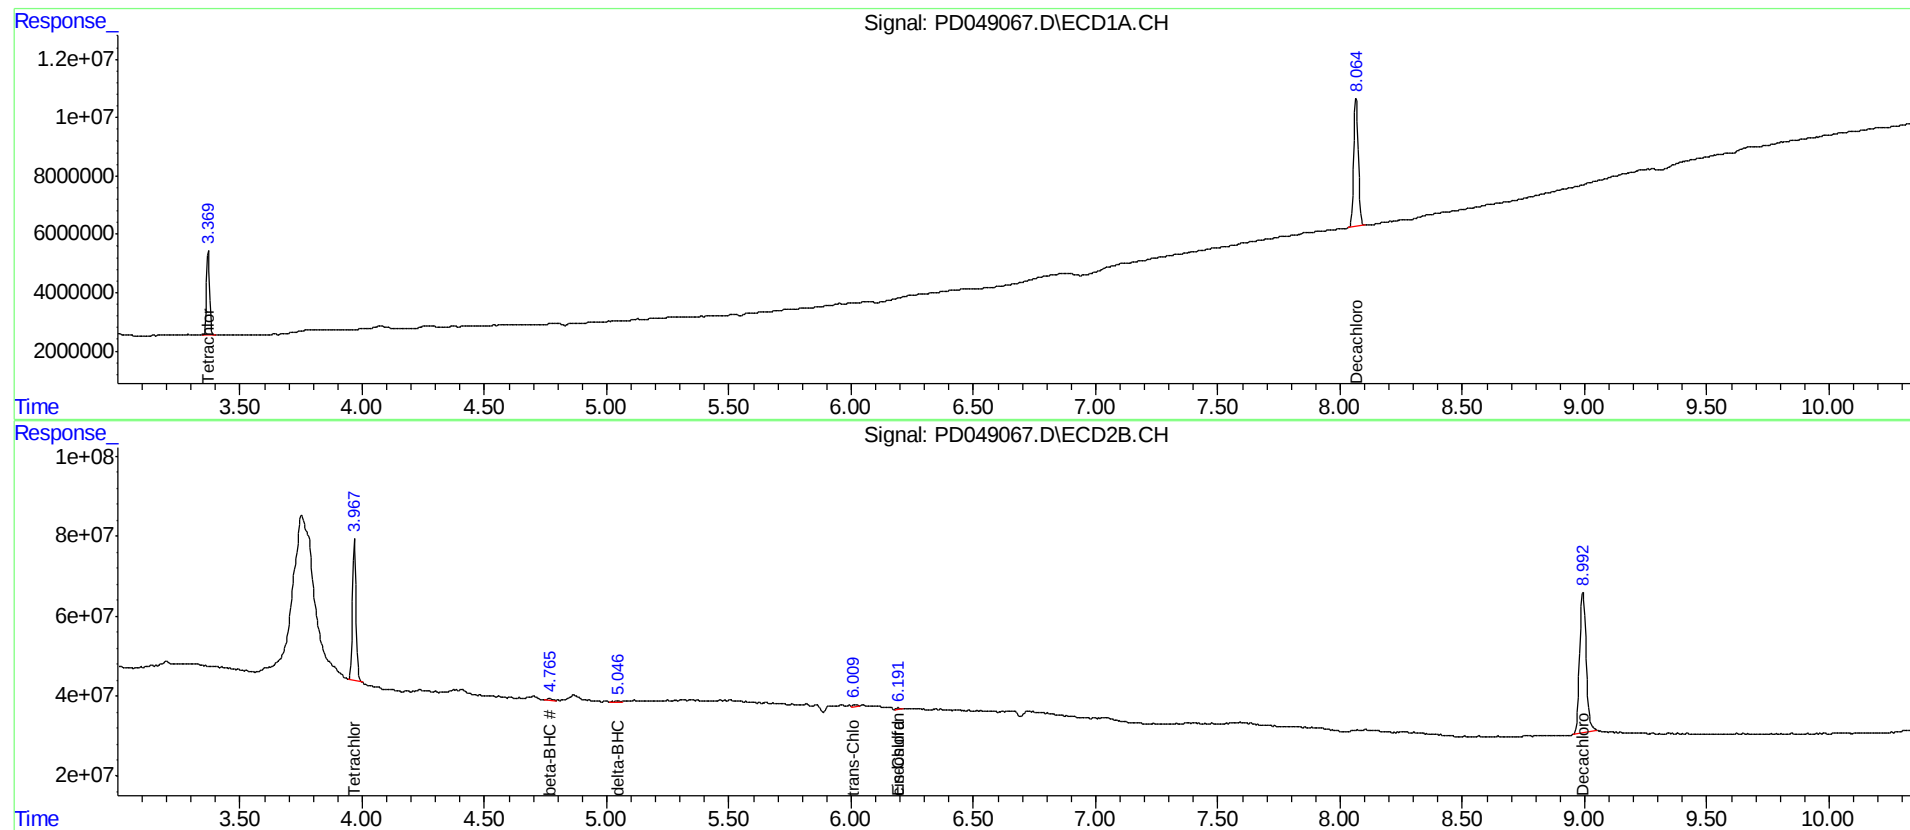


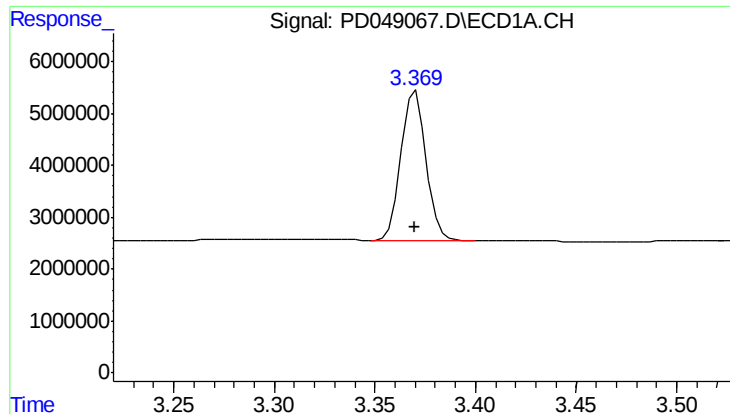

#1 Tetrachloro-m-xylene


R.T.: 3.370 min
Delta R.T.: 0.000 min
Response: 24910698
Conc: 20.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK15

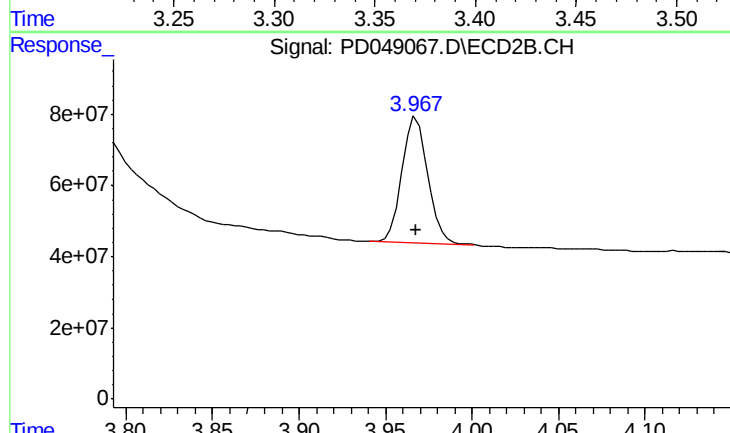


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: 0.000 min
Response: 365801665
Conc: 20.80 ng/ml

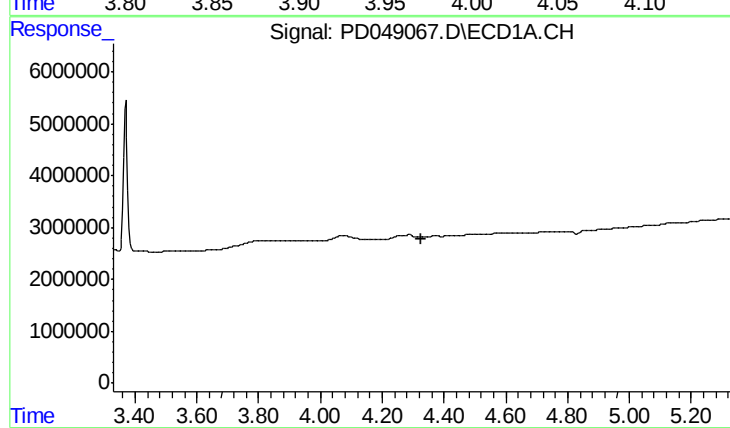


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.327 min
Response: 0
Conc: N.D.

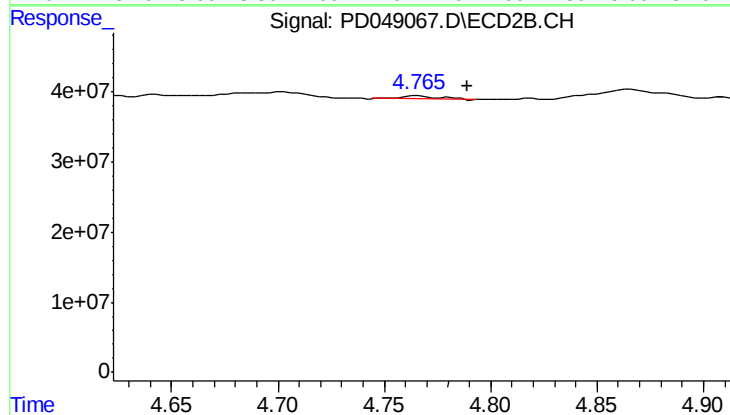

#6 beta-BHC


R.T.: 4.766 min
Delta R.T.: -0.023 min
Response: 6780284
Conc: 0.65 ng/ml

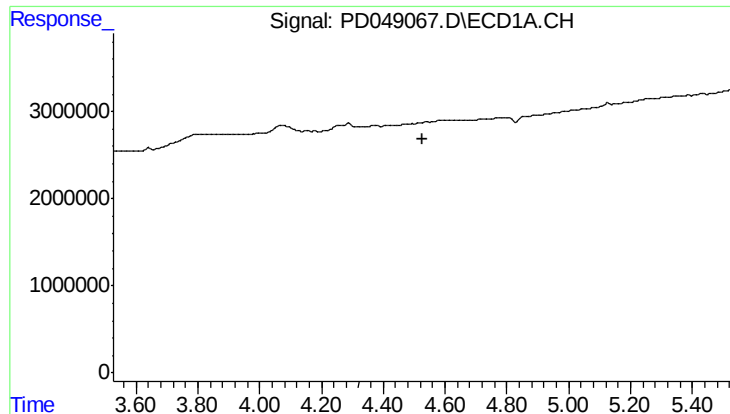

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.526 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK15

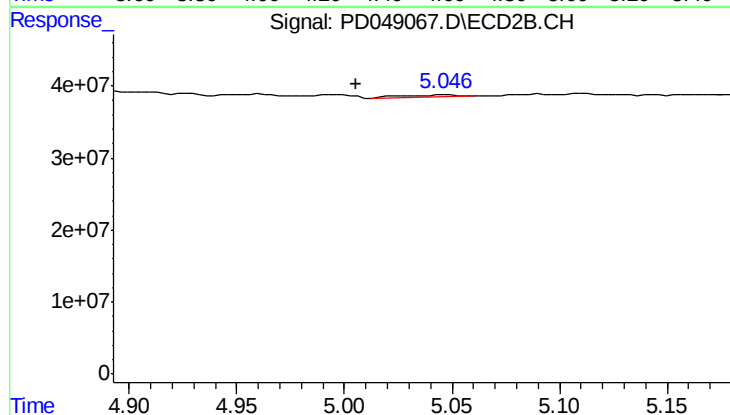


#7 delta-BHC

R.T.: 5.048 min
Delta R.T.: 0.042 min
Response: 5394362
Conc: 0.24 ng/ml

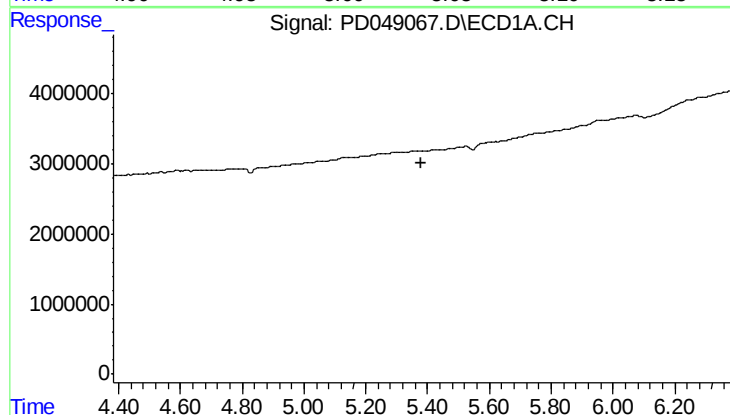


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.380 min
Response: 0
Conc: N.D.

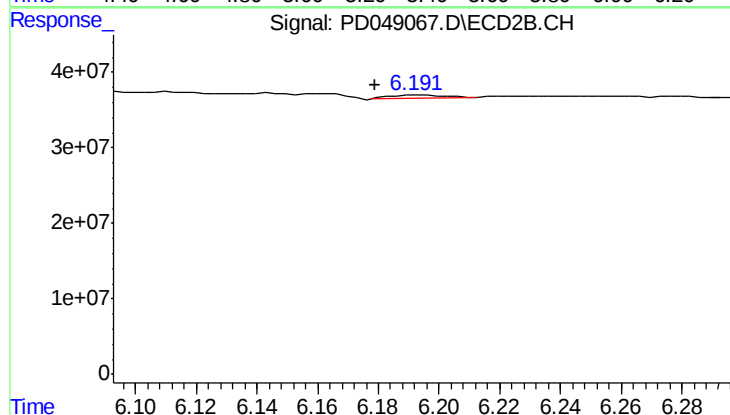

#9 Endosulfan I


R.T.: 6.193 min
Delta R.T.: 0.014 min
Response: 4687230
Conc: 0.22 ng/ml

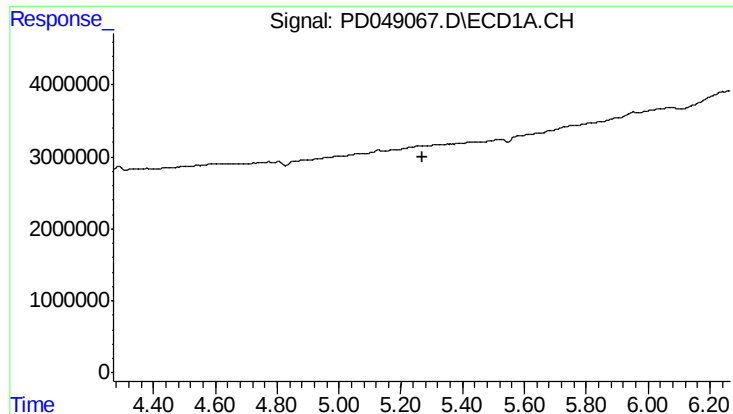

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.270 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK15

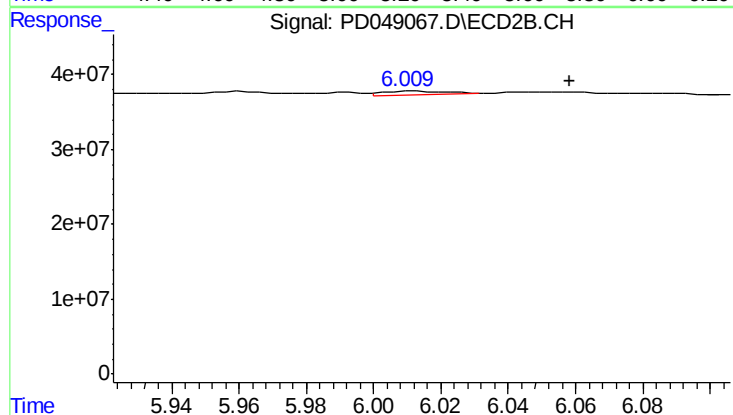


#10 trans-Chlordane

R.T.: 6.012 min
Delta R.T.: -0.046 min
Response: 4304696
Conc: 0.19 ng/ml

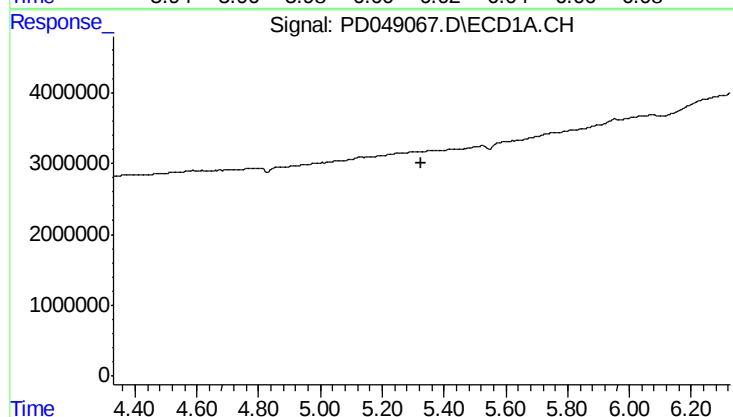


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

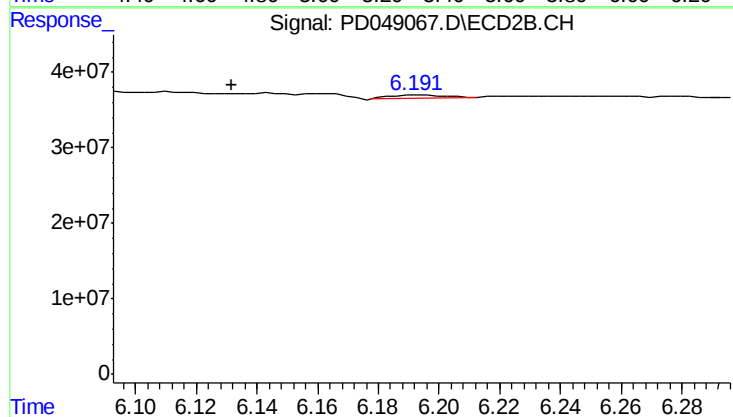

#11 cis-Chlordane


R.T.: 6.193 min
Delta R.T.: 0.062 min
Response: 4687230
Conc: 0.20 ng/ml

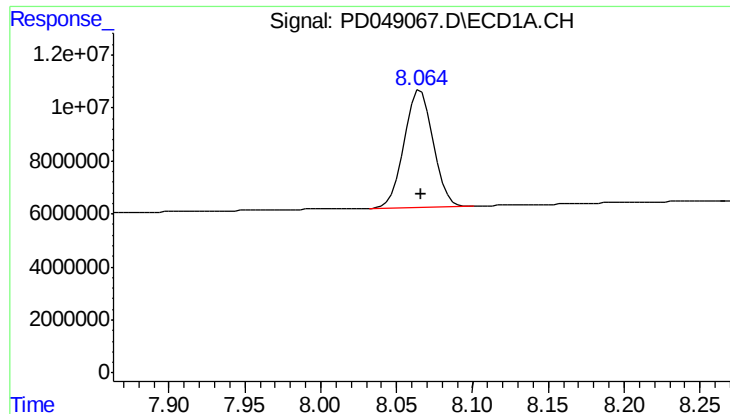

#27 Decachlorobiphenyl

R.T.: 8.066 min
Delta R.T.: 0.000 min
Response: 57995617
Conc: 40.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK15

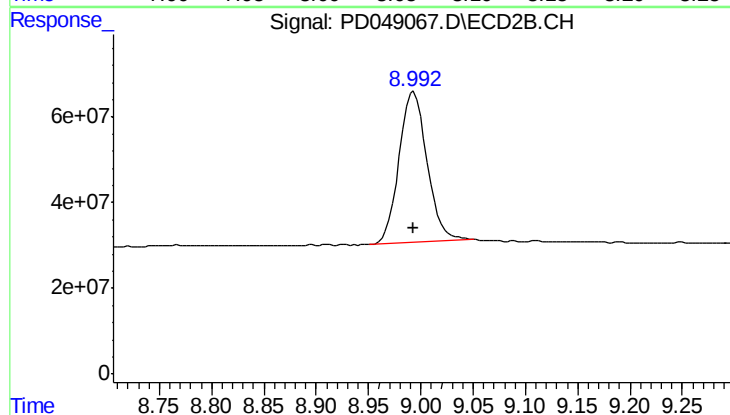

#27 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: 0.000 min
Response: 654378790
Conc: 40.42 ng/ml