

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
 Data File : PD065442.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2021 00:29
 Operator : AR\AJ
 Sample : INDA601
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 02:02:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 28 01:59:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.014	169.5E6	1192.2E6	156.902	153.559
27)	SA Decachlor...	8.238	9.084	389.4E6	1426.6E6	301.721	298.759
Target Compounds							
2)	A alpha-BHC	3.935	4.409	260.2E6	1817.4E6	167.082	160.406
3)	MA gamma-BHC...	4.219	4.695	241.2E6	1660.3E6	162.890	158.592
4)	MA Heptachlor	4.516	5.199	228.5E6	1509.3E6	158.824	155.149
9)	A Endosulfan I	5.545	6.251	192.0E6	1092.7E6	155.967	153.128
13)	MA Dieldrin	5.788	6.509	434.4E6	2356.4E6	325.635	313.557
14)	MA Endrin	6.046	6.728	383.9E6	1937.2E6	323.241	312.887
16)	A 4,4'-DDD	6.167	6.850	356.9E6	1877.7E6	323.502	311.979
17)	MA 4,4'-DDT	6.407	7.148	386.6E6	1922.0E6	326.755	316.119
20)	A Methoxychlor	6.953	7.608	929.5E6	3858.3E6	1526.100	1447.135

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
Data File : PD065442.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2021 00:29
Operator : AR\AJ
Sample : INDA601
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 02:02:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 28 01:59:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

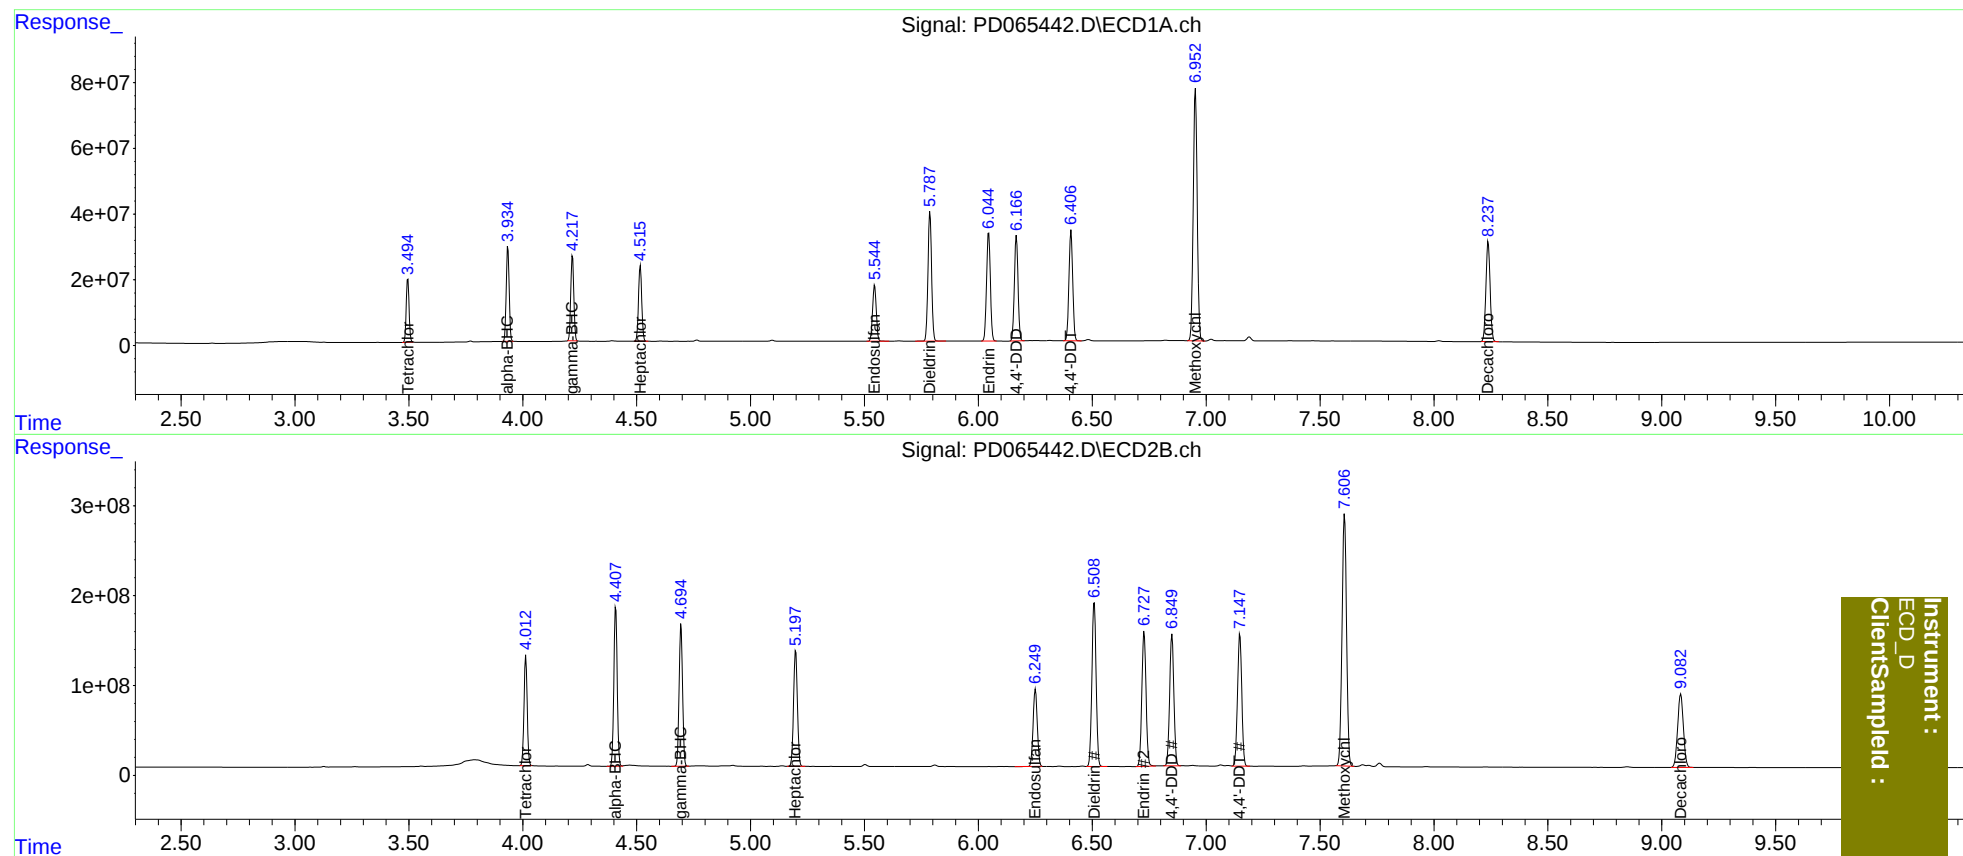

Instrument :
ECD_D
ClientSampled :