

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
 Data File : PD065434.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2021 22:39
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA2087

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 02:12:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 28 01:59:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.495	4.013	11916798	85852512	10.951	10.915
27)	SA Decachlor...	8.239	9.083	30233446	110.5E6	23.020	22.652
Target Compounds							
2)	A alpha-BHC	3.935	4.408	15490852	119.4E6	10.079	10.515
3)	MA gamma-BHC...	4.218	4.694	15354078	111.7E6	10.443	10.625
4)	MA Heptachlor	4.516	5.198	15720502	106.6E6	10.858	10.811
9)	A Endosulfan I	5.544	6.251	13716692	79645822	11.017	10.971
13)	MA Dieldrin	5.787	6.509	27750089	162.5E6	20.846	21.397
14)	MA Endrin	6.045	6.728	25123059	134.3E6	21.107	21.429
16)	A 4,4'-DDD	6.167	6.850	22907954	129.2E6	20.789	21.237
17)	MA 4,4'-DDT	6.407	7.148	24398805	129.5E6	20.677	21.138
20)	A Methoxychlor	6.953	7.607	69285740	318.6E6	111.469	115.069

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
Data File : PD065434.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2021 22:39
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 43 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 02:12:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 28 01:59:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

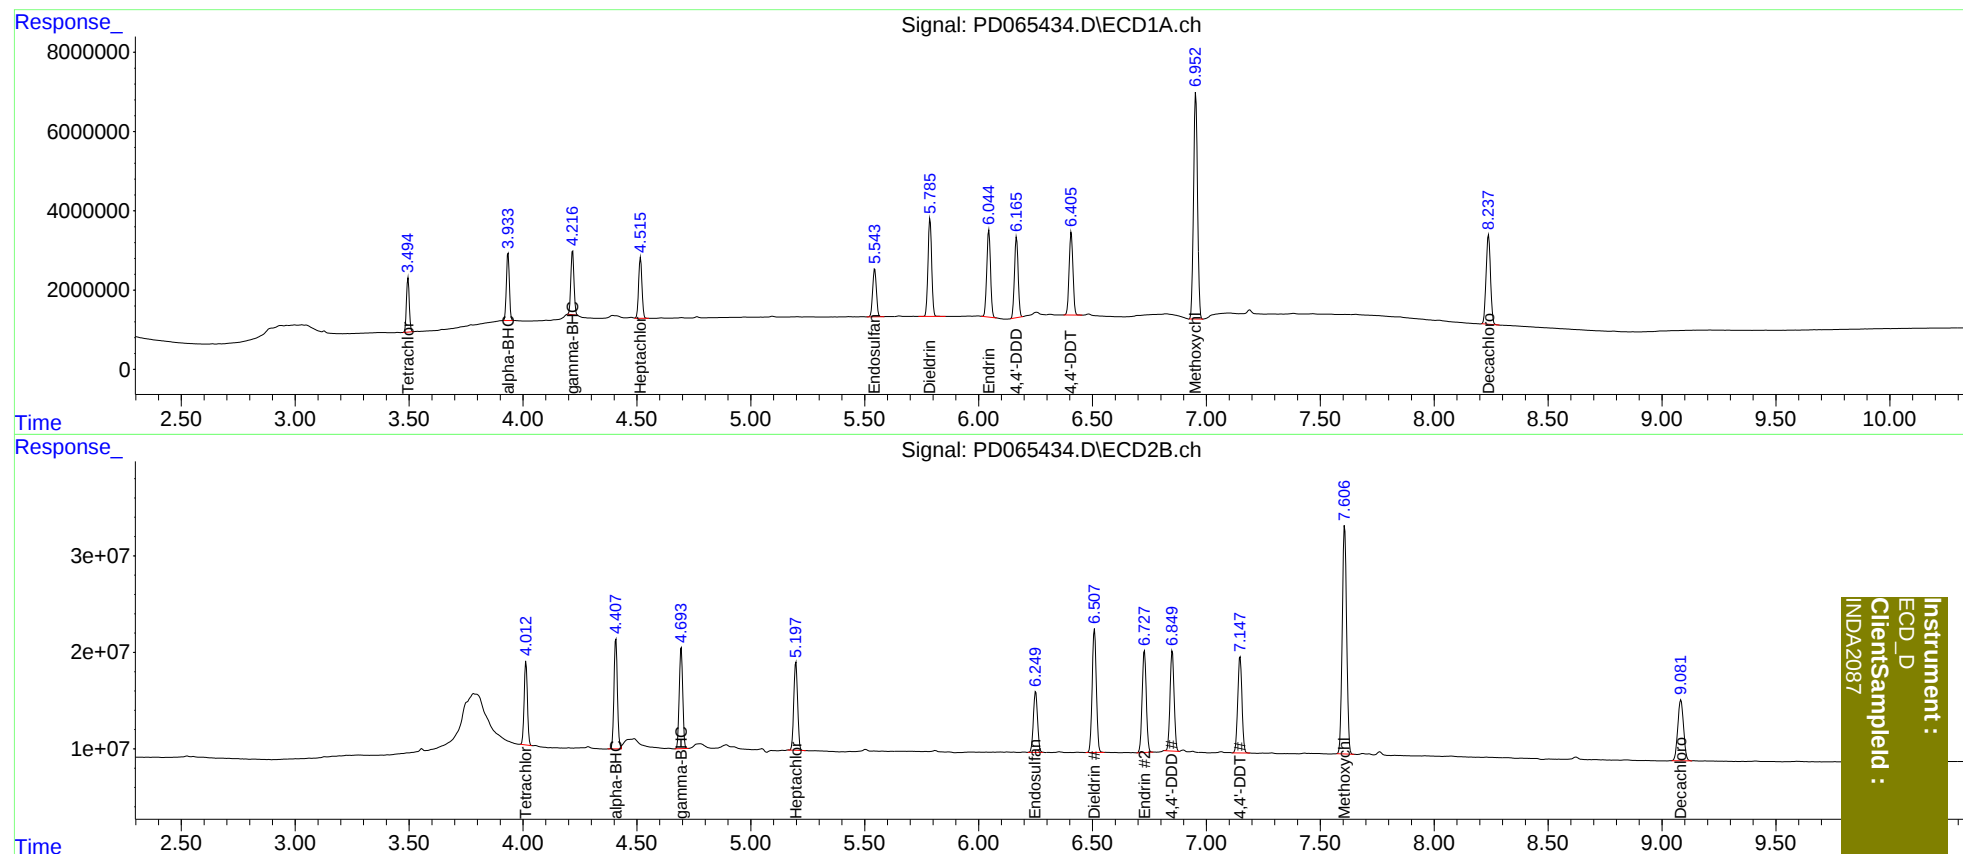

Instrument :
ECD_D
ClientSampled :
INDA2087