

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
 Data File : PD065447.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2021 01:38
 Operator : AR\AJ
 Sample : PB138667BS
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS667

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 06:45:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 28 02:37:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.014	19136263	141.6E6	17.159	17.603
27)	SA Decachlor...	8.239	9.084	48161176	177.9E6	35.190	35.379
Target Compounds							
2)	A alpha-BHC	3.935	4.408	6239356	48897629	4.030	4.247
3)	MA gamma-BHC...	4.218	4.694	6570849	46188853	4.386	4.322
4)	MA Heptachlor	4.516	5.198	6699030	47231407	4.515	4.689
5)	MB Aldrin	4.764	5.504	6321386	44129084	4.507	4.660
6)	B beta-BHC	4.466	4.870	3689565	29098377	5.043	5.633
7)	B delta-BHC	4.670	5.087	2297615	20083524	1.536	1.917
8)	B Heptachlo...	5.206	5.893	6270924	36829117	4.734	4.585
9)	A Endosulfan I	5.545	6.251	5900002	33943029	4.619	4.569
10)	B trans-Chl...	5.431	6.127	6327728	36550424	4.677	4.521
11)	B cis-Chlor...	5.490	6.198	6277755	36843461	4.690	4.684
12)	B 4,4'-DDE	5.652	6.356	11009674	68479650	8.930	9.295
13)	MA Dieldrin	5.788	6.509	12027971	70532402	8.919	9.114
14)	MA Endrin	6.045	6.728	11038834	57583526	9.112	9.064
15)	B Endosulfa...	6.317	6.941	11377092	61018696	9.211	9.397
16)	A 4,4'-DDD	6.168	6.850	9699539	56574046	8.710	9.178
17)	MA 4,4'-DDT	6.407	7.148	10236417	54722093	8.596	8.817
18)	B Endrin al...	6.486	7.065	10484879	52759188	10.530	10.280
19)	B Endosulfa...	6.697	7.288	10442915	49016080	8.284	7.944
20)	A Methoxychlor	6.954	7.607	30736375	142.2E6	48.067	49.540
21)	B Endrin ke...	7.191	7.761	14510163	67816378	9.599	9.634

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
Data File : PD065447.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2021 01:38
Operator : AR\AJ
Sample : PB138667BS
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 06:45:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 28 02:37:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

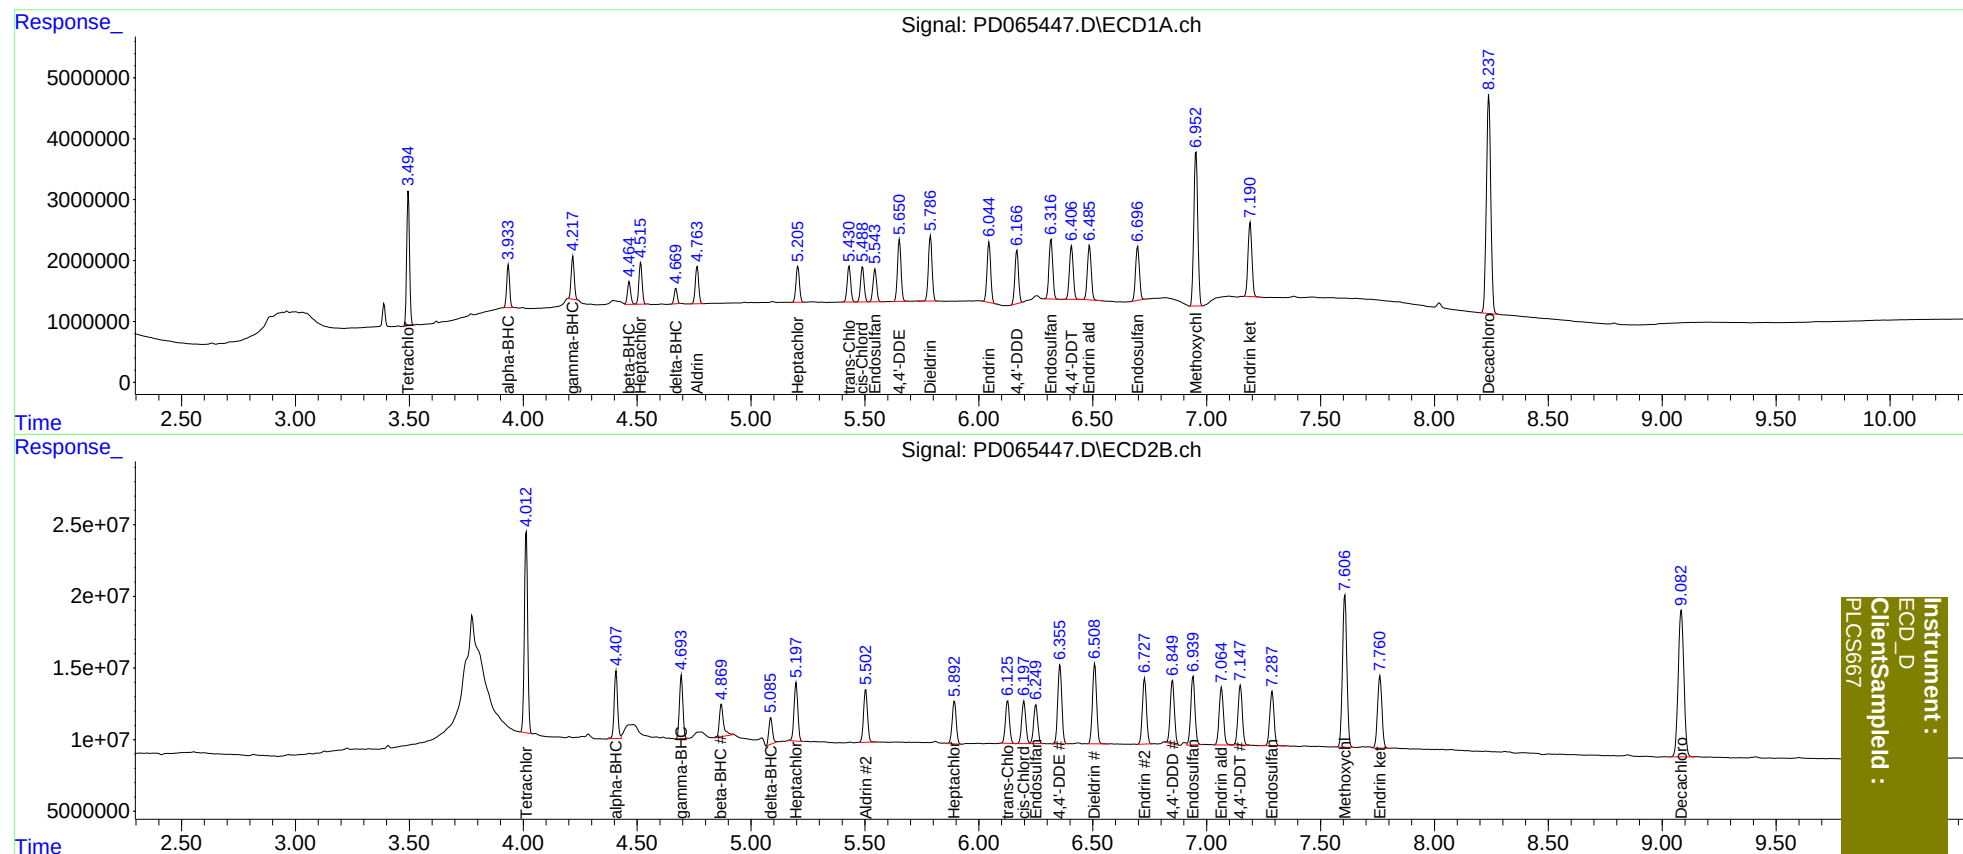

Instrument :
ECD_D
ClientSampled :
PLCS667