

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
 Data File : PD065452.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2021 02:47
 Operator : AR\AJ
 Sample : M3487-05MSD 10X
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AB8MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 06:47:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 28 02:37:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.014	21109694	152.4E6	18.929	18.940
27)	SA Decachlor...	8.239	9.083	53185290	200.4E6	38.861	39.839
Target Compounds							
2)	A alpha-BHC	3.935	4.409	77966982	566.0E6	50.357	49.159
3)	MA gamma-BHC...	4.219	4.695	73759388	523.0E6	49.233	48.936
4)	MA Heptachlor	4.517	5.199	68766503	468.1E6	46.346	46.474
5)	MB Aldrin	4.765	5.504	65688236	435.8E6	46.832	46.016
6)	B beta-BHC	4.466	4.871	33061961	230.5E6	45.191	44.613
7)	B delta-BHC	4.671	5.088	73675752	490.5E6	49.254	46.808
8)	B Heptachlo...	5.207	5.893	63845551	372.2E6	48.202	46.337
9)	A Endosulfan I	5.545	6.252	60274402	352.9E6	47.191	47.511
10)	B trans-Chl...	5.431	6.127	64237151	383.7E6	47.483	47.460
11)	B cis-Chlor...	5.490	6.199	63140271	372.6E6	47.174	47.368
12)	B 4,4'-DDE	5.653	6.357	123.3E6	725.4E6	100.008	98.471
13)	MA Dieldrin	5.788	6.509	132.0E6	751.0E6	97.866	97.047
14)	MA Endrin	6.046	6.728	118.7E6	627.7E6	97.947	98.800
15)	B Endosulfa...	6.318	6.941	117.8E6	621.7E6	95.401	95.739
16)	A 4,4'-DDD	6.168	6.851	110.4E6	607.0E6	99.123	98.473
17)	MA 4,4'-DDT	6.408	7.148	117.5E6	616.7E6	98.632	99.361
18)	B Endrin al...	6.486	7.065	102.7E6	538.4E6	103.111	104.908
19)	B Endosulfa...	6.698	7.288	119.9E6	601.1E6	95.138	97.411
20)	A Methoxychlor	6.954	7.607	309.2E6	1385.3E6	483.514	482.651
21)	B Endrin ke...	7.192	7.761	150.1E6	700.5E6	99.270	99.517

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
Data File : PD065452.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2021 02:47
Operator : AR\AJ
Sample : M3487-05MSD 10X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 06:47:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 28 02:37:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

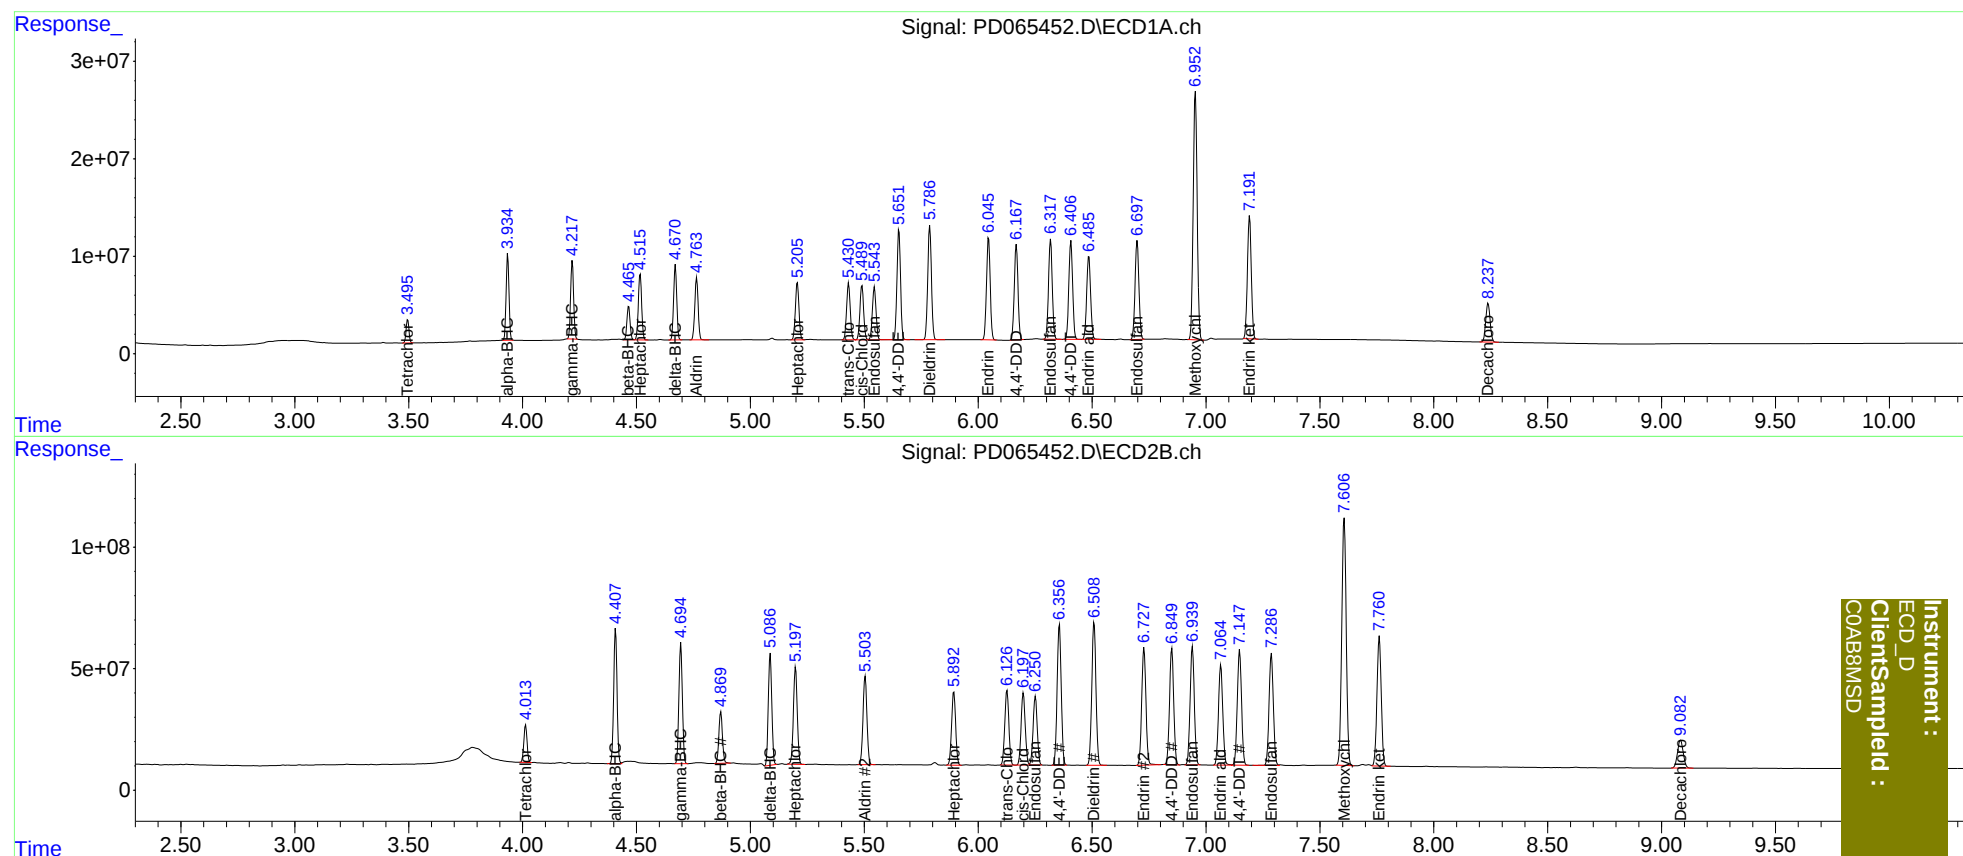

Instrument :
ECD_D
ClientSampled :
COA8B8MSD