

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
 Data File : PD065454.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2021 03:15
 Operator : AR\AJ
 Sample : PB138773BS
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS773

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 06:47:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 28 02:37:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.014	19097231	141.3E6	17.124	17.563
27)	SA Decachlor...	8.239	9.084	48079624	178.3E6	35.130	35.457
Target Compounds							
2)	A alpha-BHC	3.935	4.409	6183142	47966230	3.994	4.166
3)	MA gamma-BHC...	4.218	4.695	6546910	46086518	4.370	4.312
4)	MA Heptachlor	4.516	5.199	6708541	46610802	4.521	4.628
5)	MB Aldrin	4.764	5.504	6253079	42974262	4.458	4.538
6)	B beta-BHC	4.466	4.871	3613300	27475381	4.939	5.319
7)	B delta-BHC	4.671	5.088	2400979	19695559	1.605	1.880
8)	B Heptachlo...	5.206	5.893	6230202	41091497	4.704	5.115
9)	A Endosulfan I	5.545	6.251	5853311	33608755	4.583	4.524
10)	B trans-Chl...	5.431	6.127	6292703	36151059	4.651	4.471
11)	B cis-Chlor...	5.490	6.199	6218857	36145152	4.646	4.595
12)	B 4,4'-DDE	5.652	6.357	10899615	67916670	8.841	9.219
13)	MA Dieldrin	5.788	6.509	11916577	70003304	8.837	9.046
14)	MA Endrin	6.045	6.728	10875266	57116329	8.977	8.991
15)	B Endosulfa...	6.317	6.941	11333245	60160281	9.176	9.265
16)	A 4,4'-DDD	6.167	6.851	9642039	56026607	8.658	9.089
17)	MA 4,4'-DDT	6.407	7.148	10126950	54074900	8.504	8.712
18)	B Endrin al...	6.486	7.065	10416596	52626689	10.462	10.254
19)	B Endosulfa...	6.697	7.288	10282672	48460807	8.157	7.854
20)	A Methoxychlor	6.953	7.607	30401769	140.6E6	47.544	48.998
21)	B Endrin ke...	7.192	7.761	14427715	67124023	9.544	9.536

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
Data File : PD065454.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2021 03:15
Operator : AR\AJ
Sample : PB138773BS
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 06:47:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 28 02:37:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

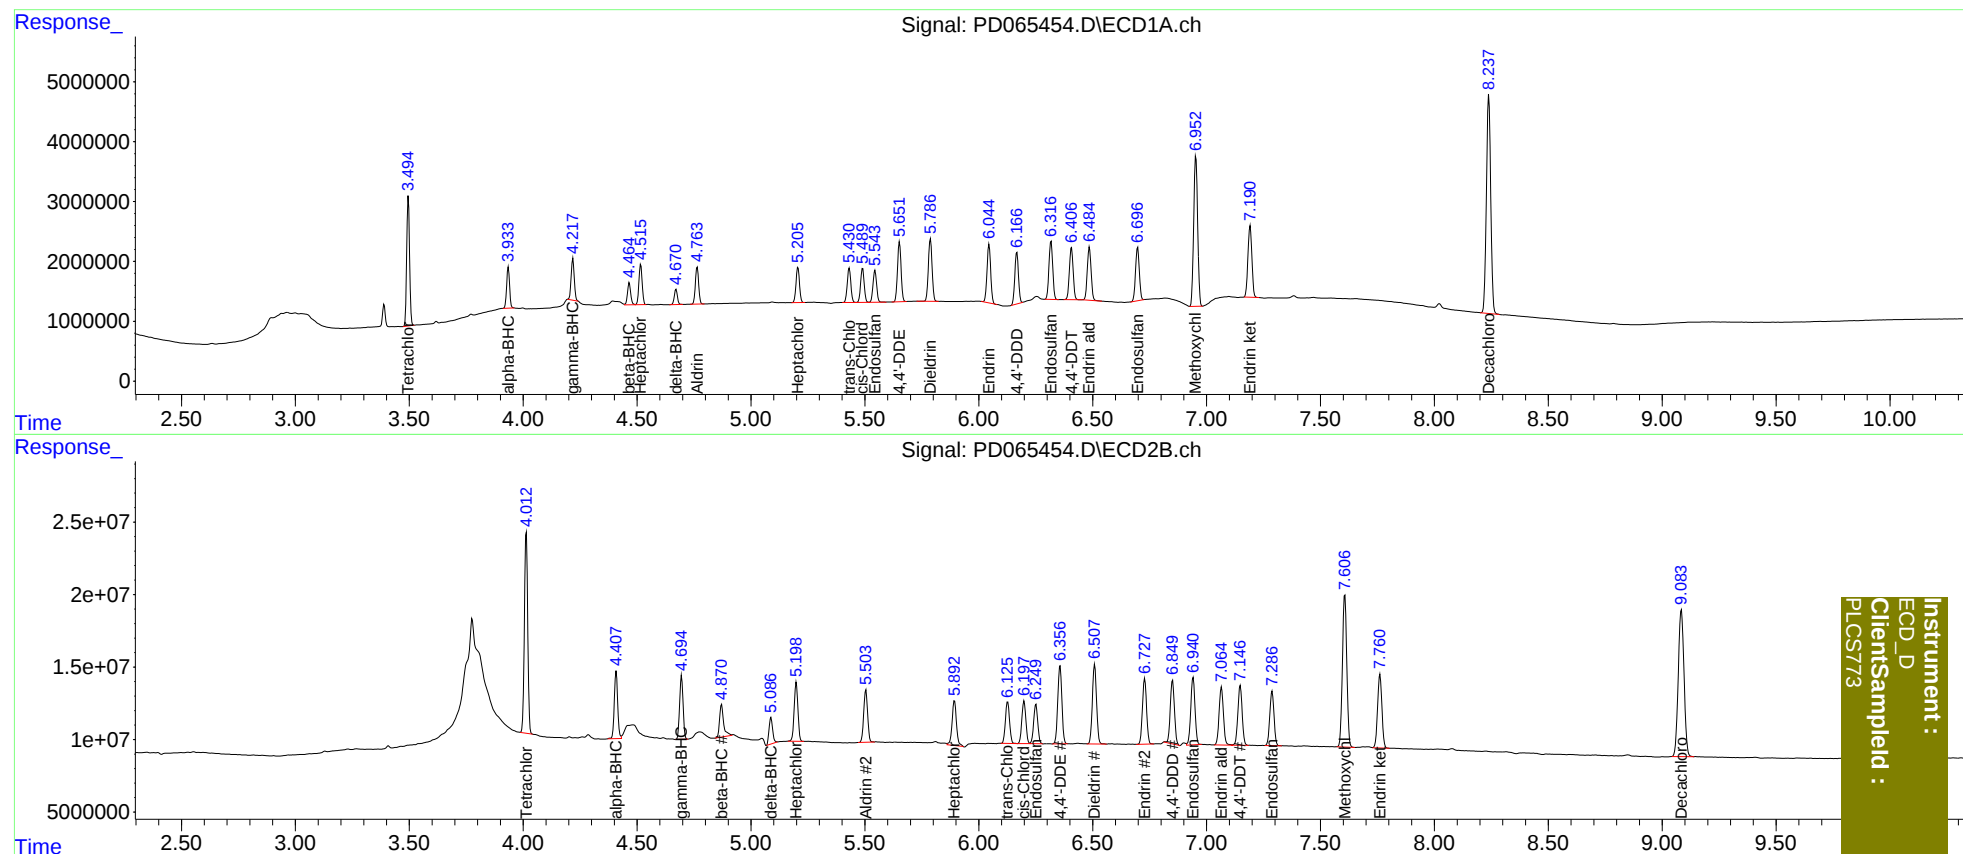

Instrument :
ECD_D
ClientSampled :
PLC5773