

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
 Data File : PD065460.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2021 04:38
 Operator : AR\AJ
 Sample : M3552-05MS 10X
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AH3MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 06:49:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 28 02:37:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	20072243	144.1E6	17.999	17.910
27)	SA Decachlor...	8.239	9.083	46605923	174.8E6	34.053	34.763
Target Compounds							
2)	A alpha-BHC	3.935	4.409	74520158	546.0E6	48.131	47.428
3)	MA gamma-BHC...	4.218	4.694	71076526	504.4E6	47.443	47.199
4)	MA Heptachlor	4.516	5.198	67489443	460.9E6	45.485	45.757
5)	MB Aldrin	4.764	5.504	63910243	427.2E6	45.565	45.112
6)	B beta-BHC	4.466	4.870	32233084	218.7E6	44.058	42.339
7)	B delta-BHC	4.671	5.087	71084251	466.8E6	47.522	44.548
8)	B Heptachlo...	5.207	5.893	61597399	354.8E6	46.505	44.160
9)	A Endosulfan I	5.545	6.251	58067881	343.9E6	45.463	46.294
10)	B trans-Chl...	5.431	6.127	62043297	373.4E6	45.862	46.188
11)	B cis-Chlor...	5.490	6.198	61229481	363.0E6	45.746	46.144
12)	B 4,4'-DDE	5.652	6.357	119.3E6	702.5E6	96.775	95.355
13)	MA Dieldrin	5.788	6.509	127.8E6	728.0E6	94.792	94.067
14)	MA Endrin	6.046	6.728	116.4E6	614.0E6	96.092	96.649
15)	B Endosulfa...	6.318	6.941	114.0E6	601.8E6	92.261	92.674
16)	A 4,4'-DDD	6.167	6.851	106.5E6	584.9E6	95.599	94.880
17)	MA 4,4'-DDT	6.407	7.148	113.6E6	597.1E6	95.398	96.197
18)	B Endrin al...	6.486	7.065	99226917	520.8E6	99.656	101.476
19)	B Endosulfa...	6.698	7.288	115.4E6	576.6E6	91.535	93.444
20)	A Methoxychlor	6.954	7.607	301.0E6	1341.2E6	470.725	467.299
21)	B Endrin ke...	7.192	7.762	144.8E6	674.3E6	95.758	95.791

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
Data File : PD065460.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2021 04:38
Operator : AR\AJ
Sample : M3552-05MS 10X
Misc :
ALS Vial : 68 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 06:49:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 28 02:37:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

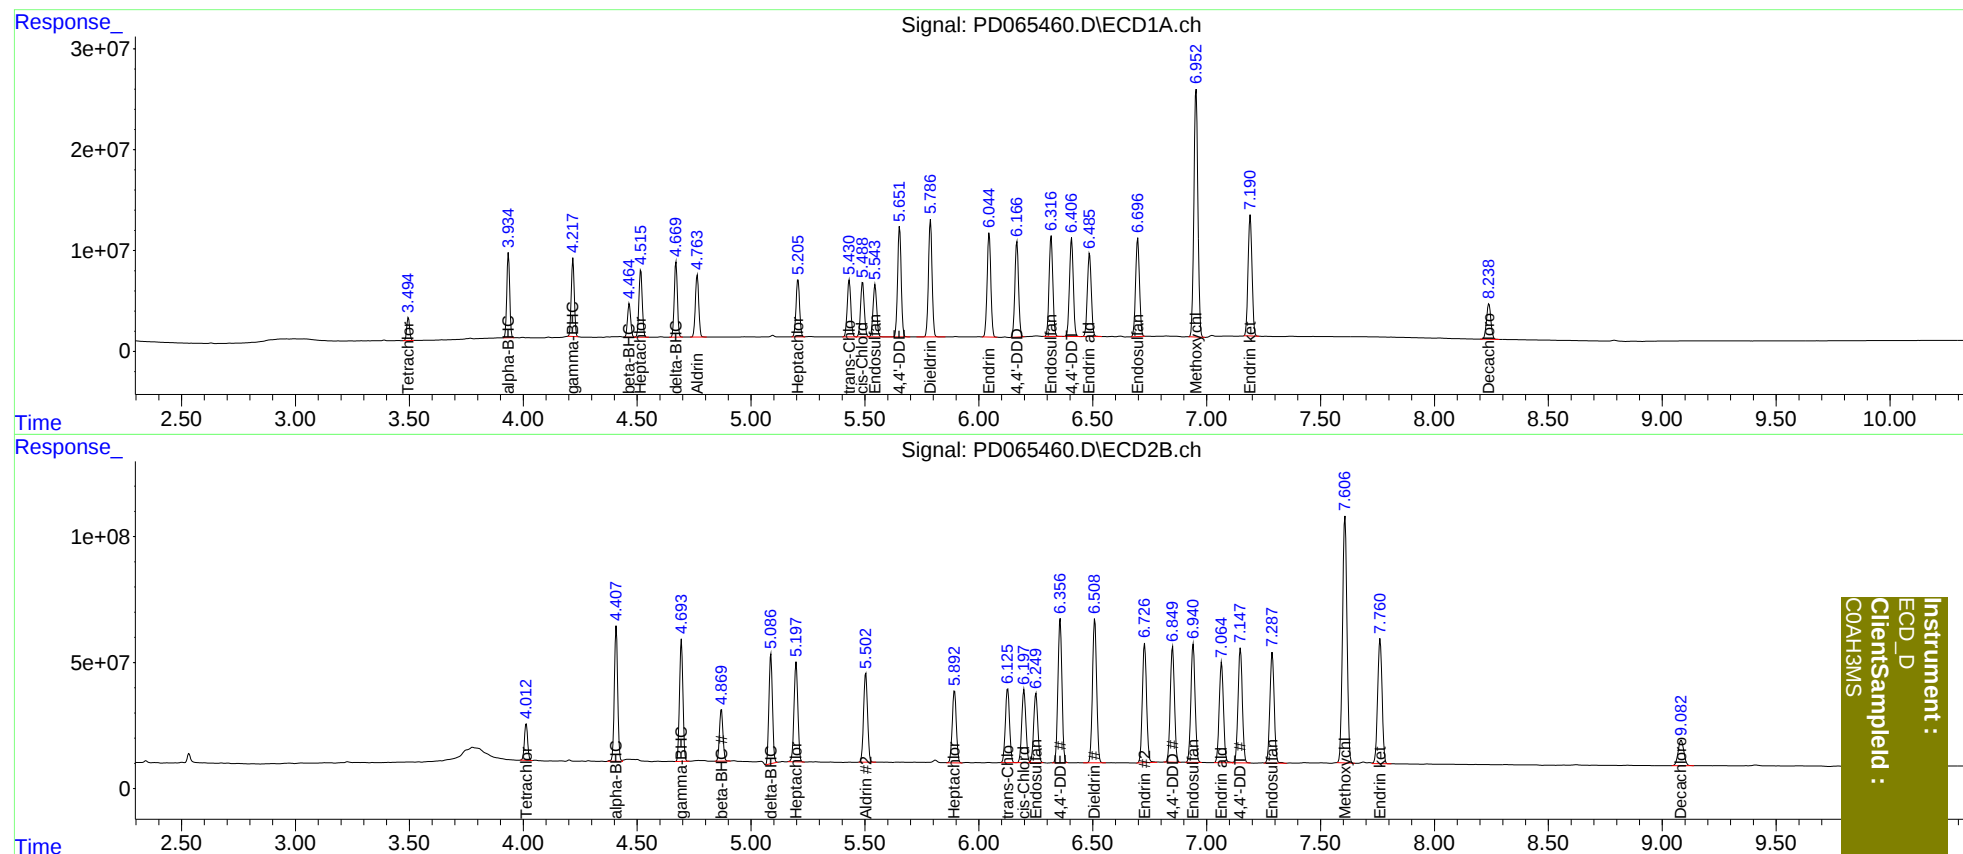

Instrument :
ECD_D
ClientSampled :
COAHMS