

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
 Data File : PD065461.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2021 04:51
 Operator : AR\AJ
 Sample : M3552-06MSD 10X
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AH3MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 06:49:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 28 02:37:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	20060704	145.9E6	17.988	18.135
27)	SA Decachlor...	8.239	9.084	48263217	181.0E6	35.264	35.990
Target Compounds							
2)	A alpha-BHC	3.935	4.408	77714907	568.1E6	50.195	49.341
3)	MA gamma-BHC...	4.218	4.695	73747699	526.2E6	49.226	49.237
4)	MA Heptachlor	4.516	5.198	70200539	481.3E6	47.313	47.781
5)	MB Aldrin	4.764	5.504	66780504	446.8E6	47.611	47.174
6)	B beta-BHC	4.466	4.870	33452272	229.3E6	45.724	44.396
7)	B delta-BHC	4.671	5.087	74051621	496.0E6	49.505	47.335
8)	B Heptachlo...	5.206	5.893	64367224	381.6E6	48.596	47.502
9)	A Endosulfan I	5.545	6.251	60621547	359.1E6	47.463	48.336
10)	B trans-Chl...	5.431	6.127	64700331	390.0E6	47.826	48.240
11)	B cis-Chlor...	5.490	6.198	63762877	378.9E6	47.639	48.170
12)	B 4,4'-DDE	5.652	6.357	124.5E6	734.7E6	101.000	99.730
13)	MA Dieldrin	5.788	6.509	133.3E6	760.0E6	98.828	98.201
14)	MA Endrin	6.045	6.728	120.7E6	639.7E6	99.668	100.701
15)	B Endosulfa...	6.318	6.941	118.8E6	628.2E6	96.168	96.741
16)	A 4,4'-DDD	6.168	6.850	110.8E6	611.5E6	99.534	99.208
17)	MA 4,4'-DDT	6.407	7.148	118.0E6	618.5E6	99.125	99.652
18)	B Endrin al...	6.486	7.065	102.9E6	542.5E6	103.346	105.699
19)	B Endosulfa...	6.698	7.288	120.3E6	604.3E6	95.423	97.931
20)	A Methoxychlor	6.953	7.608	311.1E6	1386.7E6	486.487	483.154
21)	B Endrin ke...	7.192	7.762	151.3E6	703.8E6	100.122	99.989

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
Data File : PD065461.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2021 04:51
Operator : AR\AJ
Sample : M3552-06MSD 10X
Misc :
ALS Vial : 69 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 06:49:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 28 02:37:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

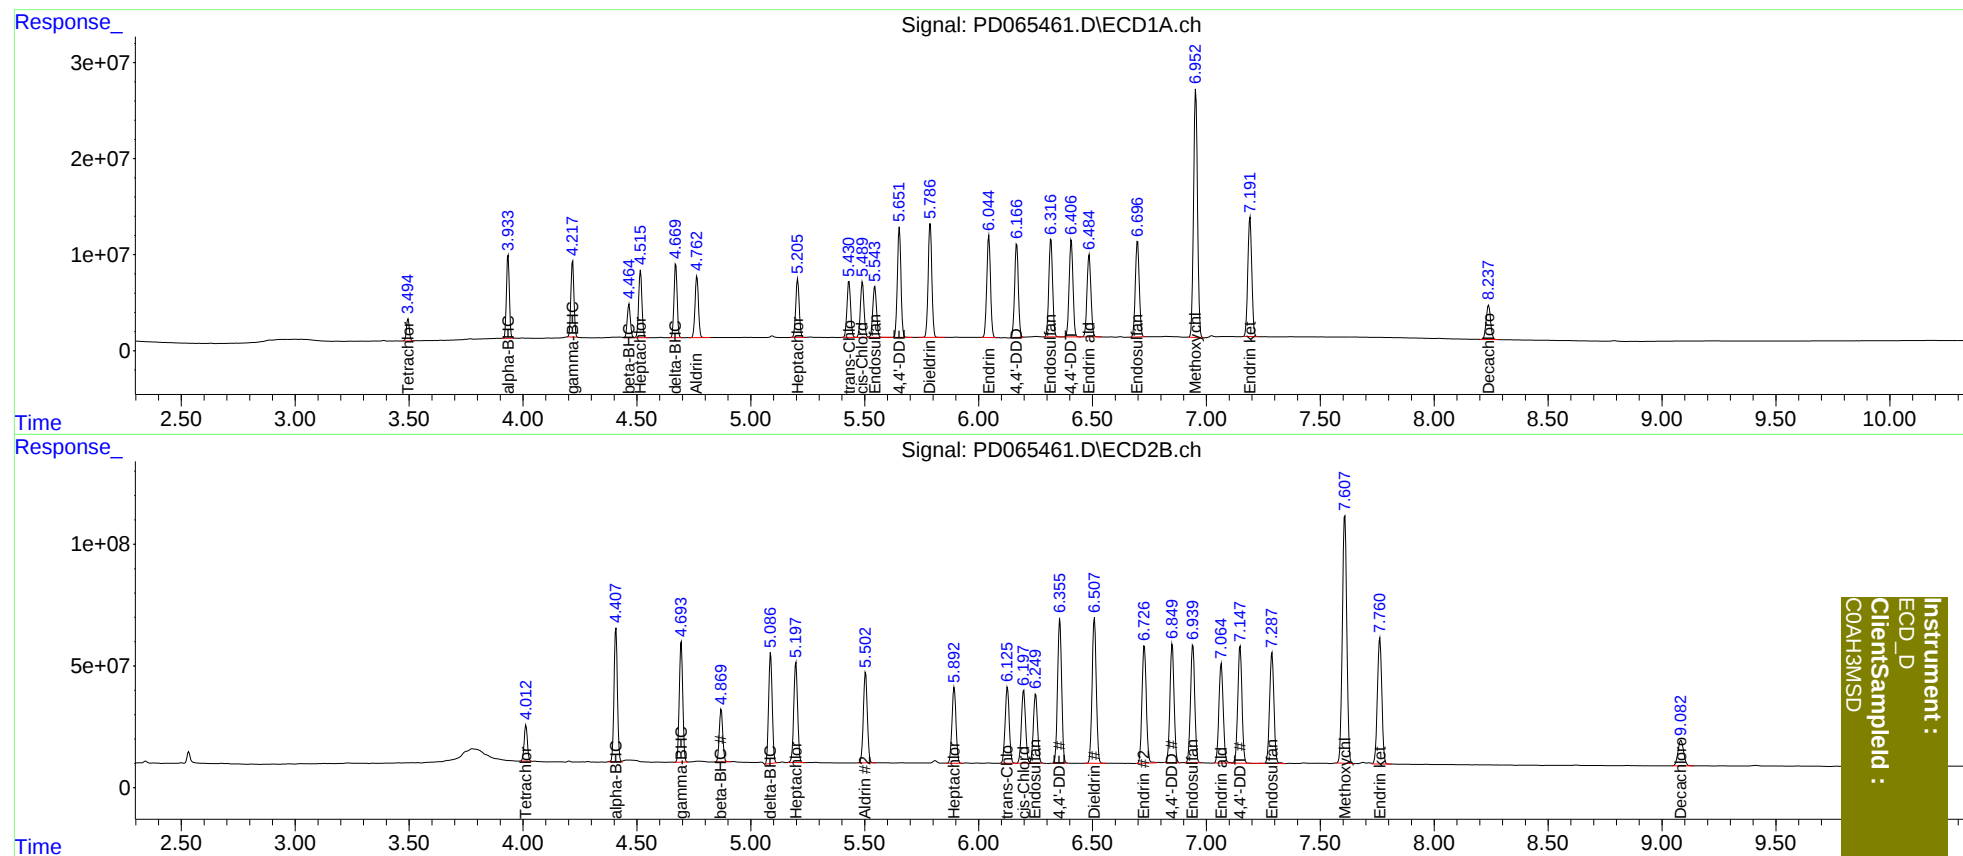

Instrument :
ECD_D
ClientSampled :
COAHMSD