

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
 Data File : PD065469.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2021 06:41
 Operator : AR\AJ
 Sample : M3553-05MS 10X
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AH7MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 07:41:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 28 02:37:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	14085742	104.1E6	12.631	12.943
27)	SA Decachlor...	8.238	9.082	29616167	109.1E6	21.640	21.689
Target Compounds							
2)	A alpha-BHC	3.935	4.408	68708437	503.6E6	44.377	43.744
3)	MA gamma-BHC...	4.218	4.695	65938940	462.9E6	44.013	43.310
4)	MA Heptachlor	4.516	5.198	50746269	354.2E6	34.201	35.162
5)	MB Aldrin	4.764	5.503	48000404	326.4E6	34.222	34.469
6)	B beta-BHC	4.466	4.870	30722888	212.5E6	41.994	41.126
7)	B delta-BHC	4.671	5.087	67103463	457.7E6	44.860	43.681
8)	B Heptachlo...	5.206	5.893	49968463	301.2E6	37.725	37.488
9)	A Endosulfan I	5.545	6.251	46855308	280.0E6	36.685	37.694
10)	B trans-Chl...	5.431	6.126	47429772	288.6E6	35.060	35.698
11)	B cis-Chlor...	5.490	6.198	47176749	281.2E6	35.247	35.748
12)	B 4,4'-DDE	5.652	6.357	88740826	533.9E6	71.977	72.469
13)	MA Dieldrin	5.788	6.509	100.3E6	582.3E6	74.347	75.246
14)	MA Endrin	6.045	6.728	92157715	497.5E6	76.070	78.309
15)	B Endosulfa...	6.317	6.941	99407961	531.4E6	80.482	81.840
16)	A 4,4'-DDD	6.167	6.850	81113594	452.9E6	72.837	73.481
17)	MA 4,4'-DDT	6.407	7.148	84418952	452.7E6	70.887	72.938
18)	B Endrin al...	6.486	7.065	90631743	482.8E6	91.023	94.064
19)	B Endosulfa...	6.697	7.287	105.2E6	530.0E6	83.479	85.889
20)	A Methoxychlor	6.953	7.607	238.2E6	1080.6E6	372.581	376.495
21)	B Endrin ke...	7.191	7.761	131.6E6	618.4E6	87.044	87.851

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
Data File : PD065469.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2021 06:41
Operator : AR\AJ
Sample : M3553-05MS 10X
Misc :
ALS Vial : 77 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 07:41:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 28 02:37:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

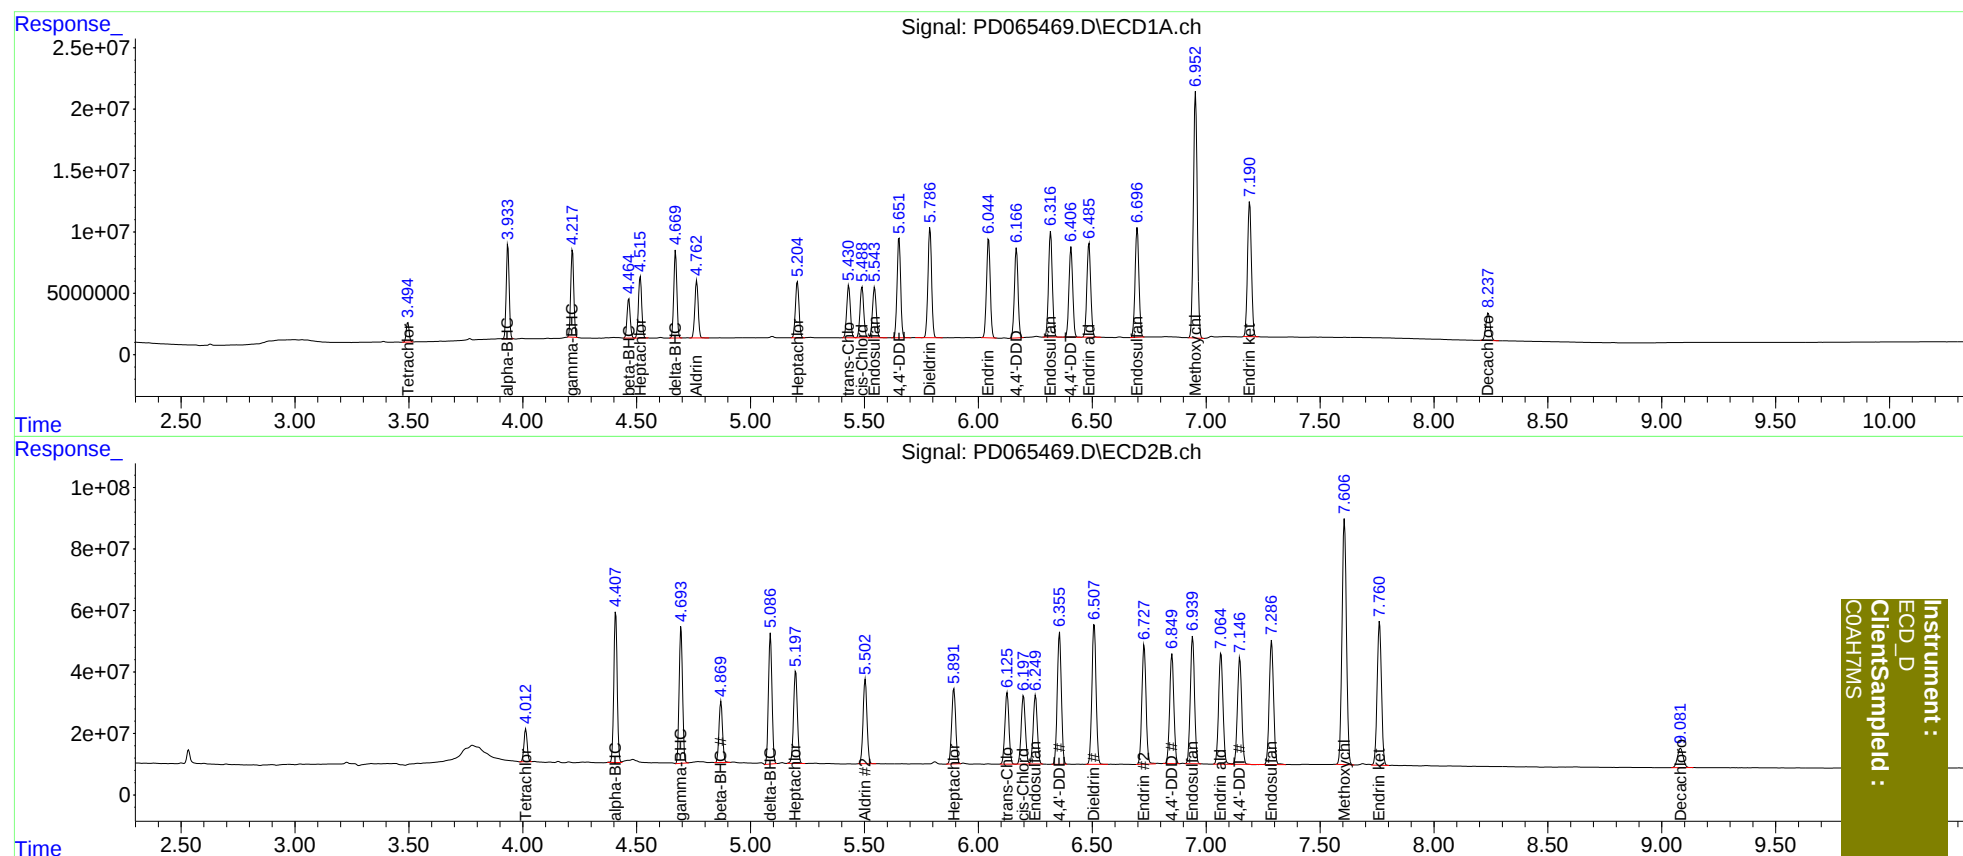

Instrument :
ECD_D
ClientSampled :
COAHTMS