

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
 Data File : PD065470.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2021 06:55
 Operator : AR\AJ
 Sample : M3553-06MSD 10X
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AH7MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 07:38:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 28 02:37:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	15986455	117.5E6	14.335	14.603
27)	SA Decachlor...	8.239	9.083	31837292	117.8E6	23.263	23.429
Target Compounds							
2)	A alpha-BHC	3.935	4.408	66632250	489.9E6	43.037	42.551
3)	MA gamma-BHC...	4.218	4.694	63910302	443.9E6	42.659	41.539
4)	MA Heptachlor	4.516	5.198	56203817	390.1E6	37.879	38.734
5)	MB Aldrin	4.764	5.503	53221043	358.9E6	37.944	37.898
6)	B beta-BHC	4.466	4.870	29514243	203.2E6	40.342	39.331
7)	B delta-BHC	4.671	5.087	64090038	441.6E6	42.846	42.147
8)	B Heptachlo...	5.206	5.893	52840427	322.8E6	39.894	40.178
9)	A Endosulfan I	5.545	6.251	49696882	296.2E6	38.909	39.868
10)	B trans-Chl...	5.431	6.126	51793225	315.0E6	38.285	38.961
11)	B cis-Chlor...	5.490	6.198	51517508	306.6E6	38.490	38.972
12)	B 4,4'-DDE	5.652	6.356	97600156	585.1E6	79.163	79.413
13)	MA Dieldrin	5.788	6.508	107.5E6	622.3E6	79.692	80.415
14)	MA Endrin	6.046	6.728	97942318	527.9E6	80.845	83.096
15)	B Endosulfa...	6.317	6.940	100.0E6	534.1E6	80.973	82.254
16)	A 4,4'-DDD	6.168	6.850	88230567	491.1E6	79.228	79.665
17)	MA 4,4'-DDT	6.408	7.148	92384074	492.0E6	77.576	79.274
18)	B Endrin al...	6.486	7.065	87776934	465.4E6	88.156	90.671
19)	B Endosulfa...	6.698	7.287	103.2E6	517.3E6	81.877	83.827
20)	A Methoxychlor	6.954	7.607	254.1E6	1142.9E6	397.388	398.189
21)	B Endrin ke...	7.191	7.760	128.3E6	603.1E6	84.878	85.672

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
Data File : PD065470.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2021 06:55
Operator : AR\AJ
Sample : M3553-06MSD 10X
Misc :
ALS Vial : 78 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 07:38:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 28 02:37:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

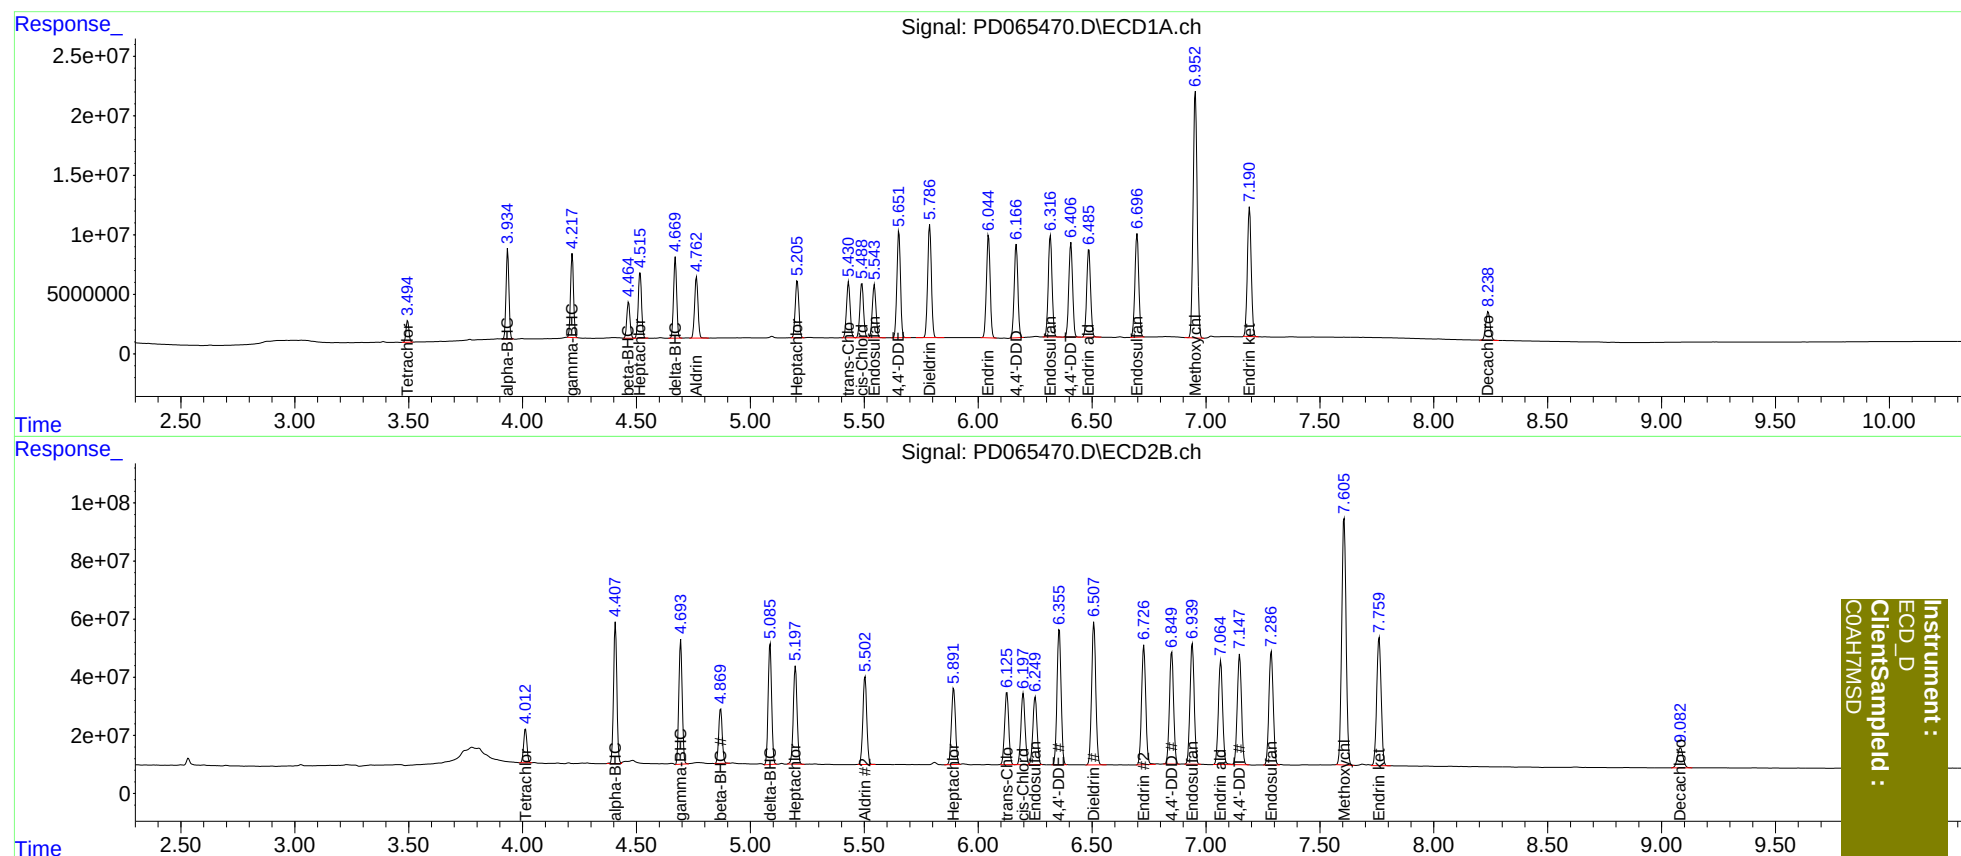

Instrument :
ECD_D
ClientSampled :
COAHTMSD