

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
 Data File : PD065424.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2021 20:21
 Operator : AR\AJ
 Sample : RESC13
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC008

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 02:39:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 28 02:37:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.014	21559494	156.5E6	19.332	19.456
2)	SA Decachlor...	8.238	9.083	53634930	198.9E6	39.189	39.555
Target Compounds							
2)	A alpha-BHC	3.935	4.408	14757823	113.7E6	9.532	9.874
3)	MA gamma-BHC...	4.218	4.695	14823241	106.1E6	9.894	9.926
4)	MA Heptachlor	4.516	5.198	14856634	101.5E6	10.013	10.078
5)	MB Aldrin	4.764	5.503	14397274	98997057	10.264	10.453
6)	B beta-BHC	4.466	4.870	7959312	56124055	10.879	10.864
7)	B delta-BHC	4.671	5.087	14472451	103.9E6	9.675	9.914
8)	B Heptachlo...	5.206	5.893	13675576	80692667	10.325	10.045
9)	A Endosulfan I	5.544	6.250	13013576	75486898	10.189	10.161
10)	B trans-Chl...	5.431	6.126	13937350	82285205	10.302	10.178
11)	B cis-Chlor...	5.490	6.198	13819984	80921426	10.325	10.287
12)	B 4,4'-DDE	5.652	6.356	24201838	147.9E6	19.630	20.070
13)	MA Dieldrin	5.787	6.508	26417729	155.3E6	19.590	20.064
14)	MA Endrin	6.045	6.728	23941538	127.7E6	19.762	20.102
15)	B Endosulfa...	6.317	6.940	25304223	134.3E6	20.487	20.689
16)	A 4,4'-DDD	6.167	6.850	21766609	122.6E6	19.546	19.886
17)	MA 4,4'-DDT	6.407	7.148	23121763	125.3E6	19.416	20.187
18)	B Endrin al...	6.486	7.065	20729166	107.0E6	20.819	20.841
19)	B Endosulfa...	6.697	7.287	25991282	127.0E6	20.619	20.579
20)	A Methoxychlor	6.953	7.607	65938810	303.4E6	103.118	105.723
21)	B Endrin ke...	7.191	7.761	31941179	149.1E6	21.130	21.177

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
Data File : PD065424.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2021 20:21
Operator : AR\AJ
Sample : RESC13
Misc :
ALS Vial : 33 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 02:39:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 28 02:37:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

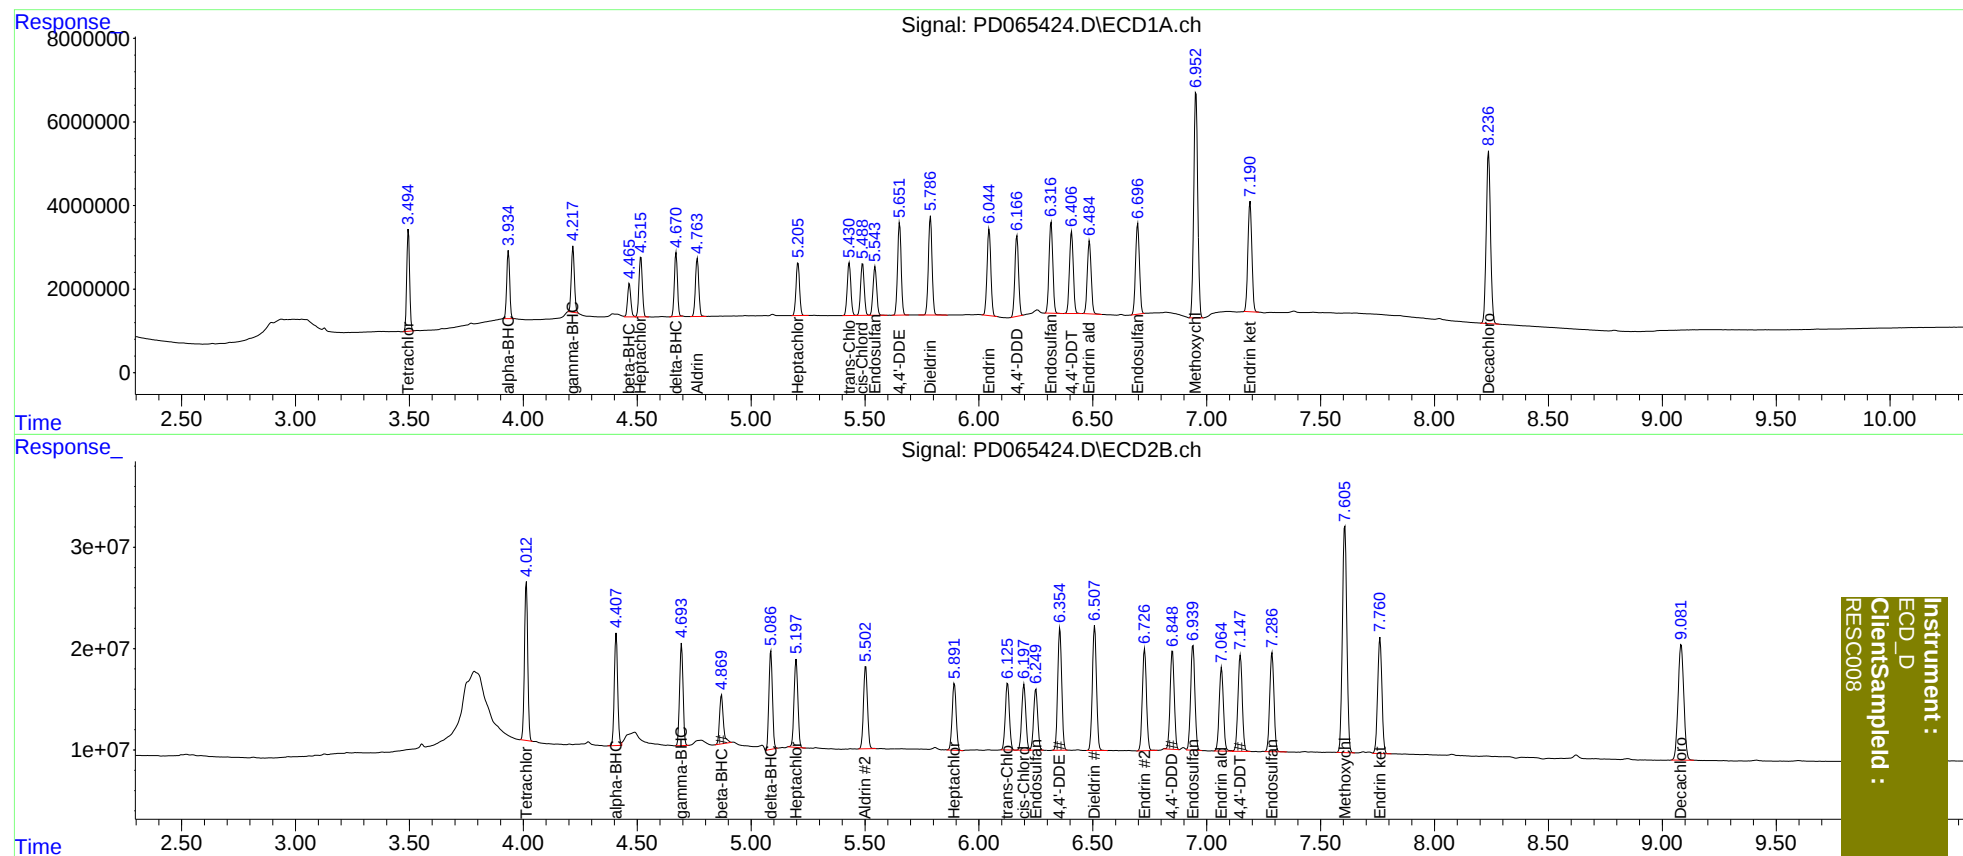

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
Data File : PD065424.D
Acq On : 27 Aug 2021 20:21
Operator : AR\AJ
Sample : RESC13
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC008

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
Title : GC Extractables
Last Update : Sat Aug 28 02:37:59 2021
Integrator: ChemStation

RT#1	RT#2	Resolution
3.496	3.935	100.00%
3.935	4.218	100.00%
4.218	4.466	100.00%
4.466	4.516	99.12%
4.516	4.671	100.00%
4.671	4.764	100.00%
4.764	5.206	100.00%
5.206	5.431	100.00%
5.431	5.490	99.40%
5.490	5.544	100.00%
5.544	5.652	100.00%
5.652	5.787	100.00%
5.787	6.045	100.00%
6.045	6.167	100.00%
6.167	6.317	100.00%
6.317	6.407	100.00%
6.407	6.486	100.00%
6.486	6.697	100.00%
6.697	6.953	100.00%
6.953	7.191	100.00%
7.191	8.238	100.00%

Signal #2


4.014	4.408	100.00%
4.408	4.695	100.00%
4.695	4.870	100.00%
4.870	5.087	100.00%
5.087	5.198	100.00%
5.198	5.503	100.00%
5.503	5.893	100.00%
5.893	6.126	100.00%
6.126	6.198	100.00%
6.198	6.250	98.91%
6.250	6.356	100.00%
6.356	6.508	100.00%
6.508	6.728	100.00%
6.728	6.850	100.00%
6.850	6.940	100.00%
6.940	7.065	100.00%
7.065	7.148	100.00%
7.148	7.287	100.00%
7.287	7.607	100.00%
7.607	7.761	100.00%
7.761	9.083	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
Data File : PD065424.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2021 20:21
Operator : AR\AJ
Sample : RESC13
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC008

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 02:39:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 28 02:37:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

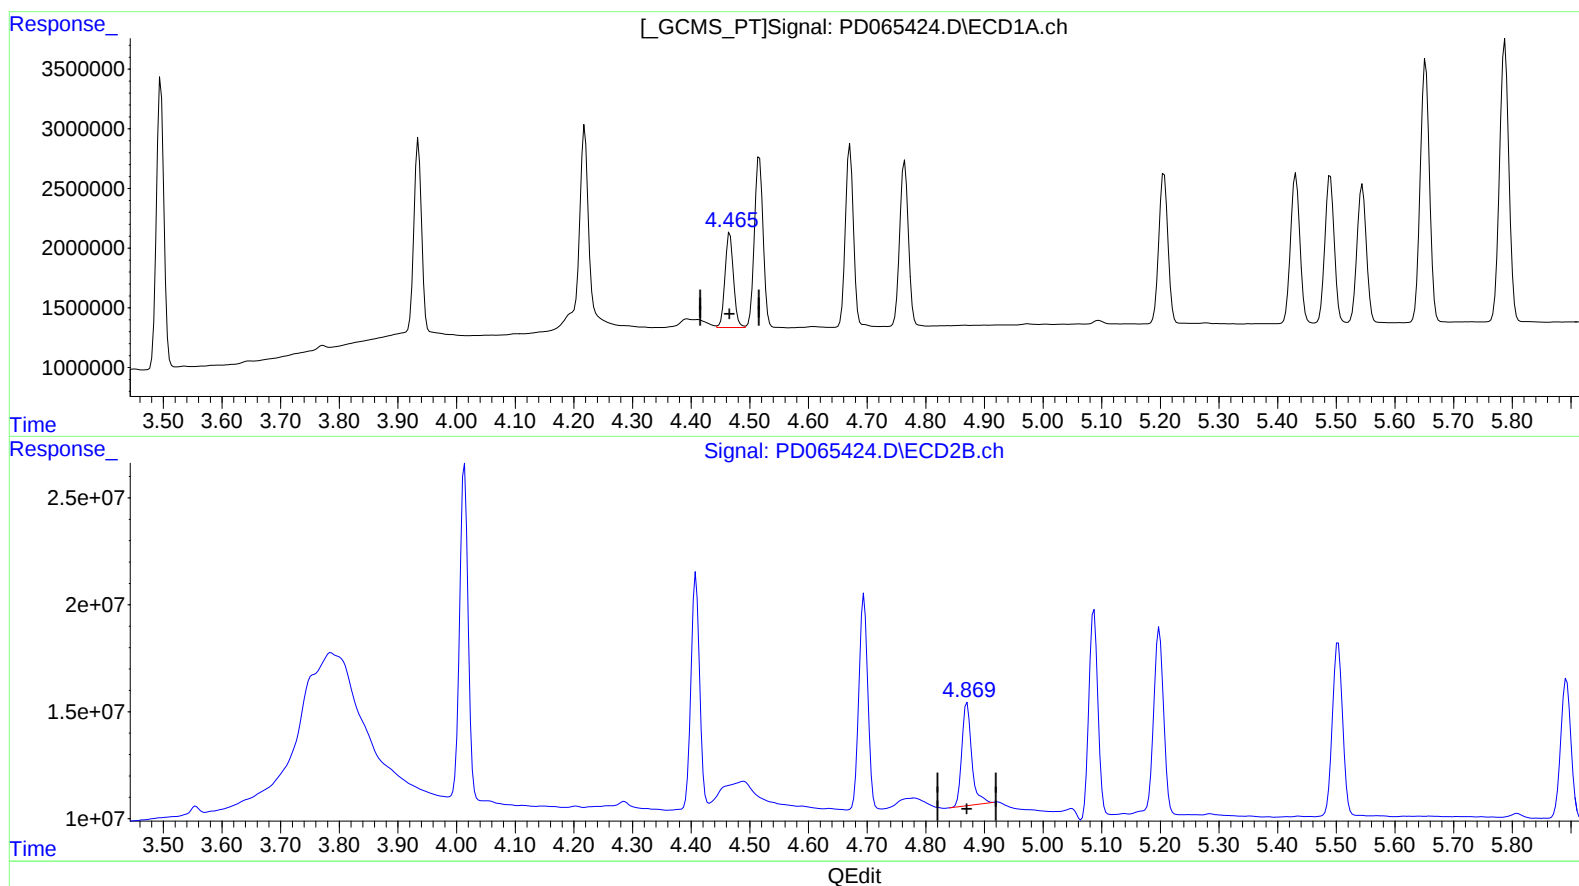

(6) beta-BHC (B)

4.466min 10.879 ng/ml

response 7959312

(6) beta-BHC #2 (B)

4.870min 10.864 ng/ml


response 56124055

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
Data File : PD065424.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2021 20:21
Operator : AR\AJ
Sample : RESC13
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC008

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 02:39:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 28 02:37:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

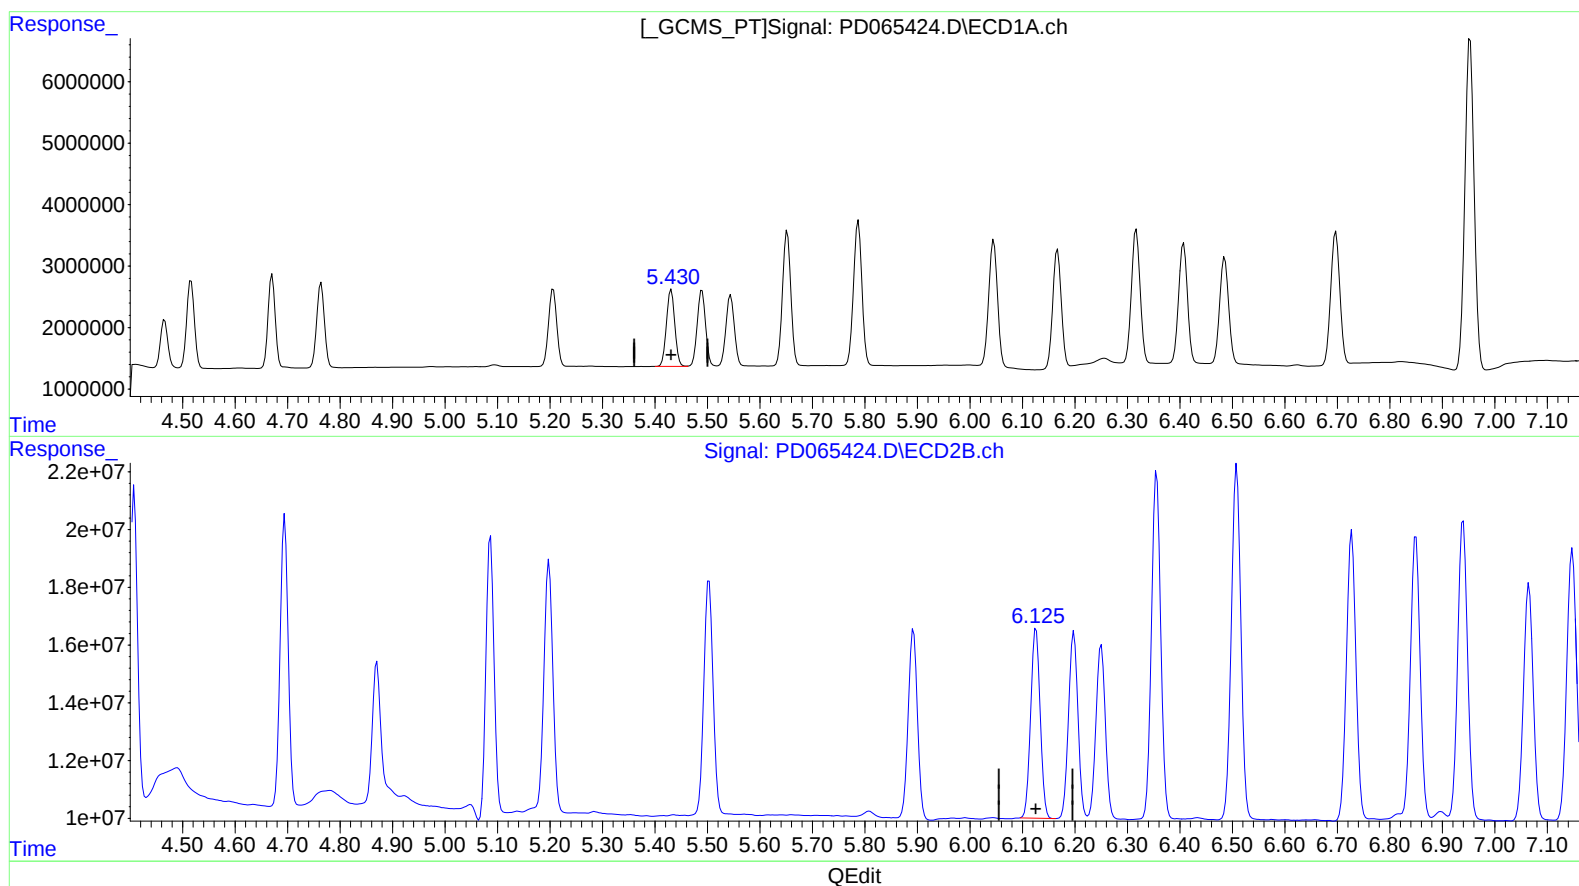

(10) trans-Chlordane (B)

5.431min 10.302 ng/ml

response 13937350

(10) trans-Chlordane #2 (B)

6.126min 10.178 ng/ml


response 82285205

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
Data File : PD065424.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2021 20:21
Operator : AR\AJ
Sample : RESC13
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC008

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 02:39:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 28 02:37:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

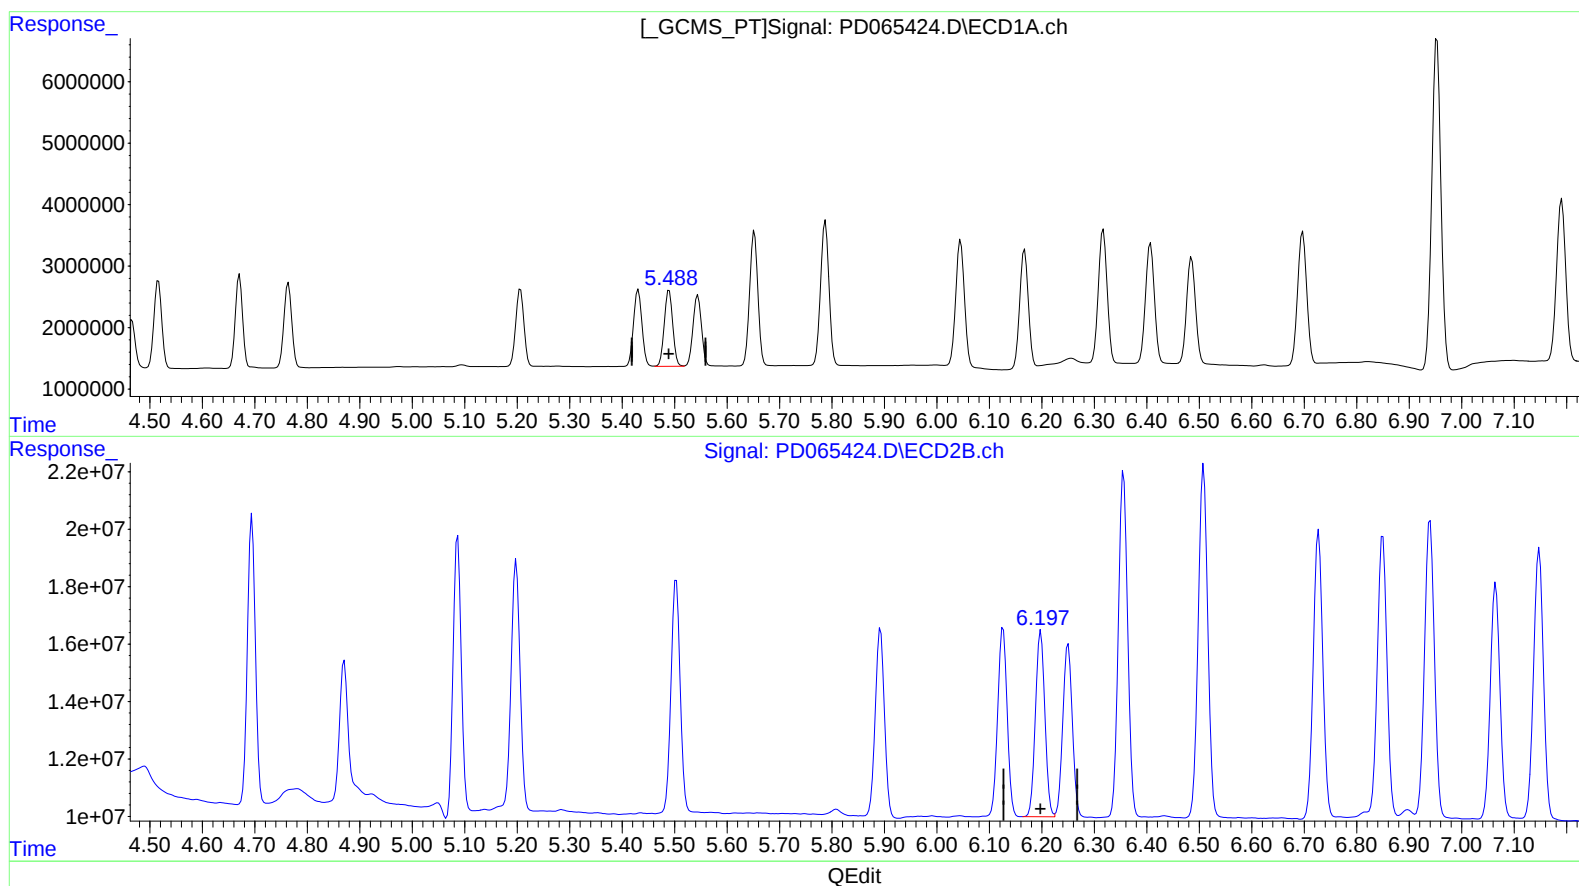

(11) cis-Chlordane (B)

5.490min 10.325 ng/ml

response 13819984

(11) cis-Chlordane #2 (B)

6.198min 10.287 ng/ml

response 80921426