

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
 Data File : PD065463.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2021 05:19
 Operator : AR\AJ
 Sample : PB138771BS
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS771

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 06:49:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 28 02:37:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	18972452	140.0E6	17.012	17.397
2)	SA Decachlor...	8.239	9.083	47616224	177.9E6	34.792	35.364
Target Compounds							
2)	A alpha-BHC	3.935	4.409	6116010	47743680	3.950	4.147
3)	MA gamma-BHC...	4.218	4.695	6357042	46186280	4.243	4.322
4)	MA Heptachlor	4.516	5.199	6696873	47154692	4.513	4.682
5)	MB Aldrin	4.764	5.504	6221968	43437919	4.436	4.587
6)	B beta-BHC	4.466	4.871	3608549	26019502	4.932	5.037
7)	B delta-BHC	4.671	5.087	2382621	20138742	1.593	1.922
8)	B Heptachlo...	5.207	5.893	6222669	36539935	4.698	4.549
9)	A Endosulfan I	5.545	6.251	5848583	33238221	4.579	4.474
10)	B trans-Chl...	5.431	6.127	6265202	36288404	4.631	4.488
11)	B cis-Chlor...	5.490	6.199	6226230	36007161	4.652	4.577
12)	B 4,4'-DDE	5.652	6.357	10962529	67784653	8.892	9.201
13)	MA Dieldrin	5.788	6.509	11876251	70095237	8.807	9.057
14)	MA Endrin	6.046	6.729	10872175	56763294	8.974	8.935
15)	B Endosulfa...	6.318	6.941	11321906	60783028	9.166	9.361
16)	A 4,4'-DDD	6.168	6.851	9675455	56856723	8.688	9.224
17)	MA 4,4'-DDT	6.407	7.148	10047374	53682320	8.437	8.649
18)	B Endrin al...	6.486	7.066	10373267	52509093	10.418	10.231
19)	B Endosulfa...	6.698	7.288	10278010	49308106	8.154	7.991
20)	A Methoxychlor	6.954	7.607	30101999	140.9E6	47.075	49.100
21)	B Endrin ke...	7.192	7.761	14412253	67231480	9.534	9.551

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083021\
Data File : PD065463.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2021 05:19
Operator : AR\AJ
Sample : PB138771BS
Misc :
ALS Vial : 71 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 06:49:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD083021TCLP-CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 28 02:37:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

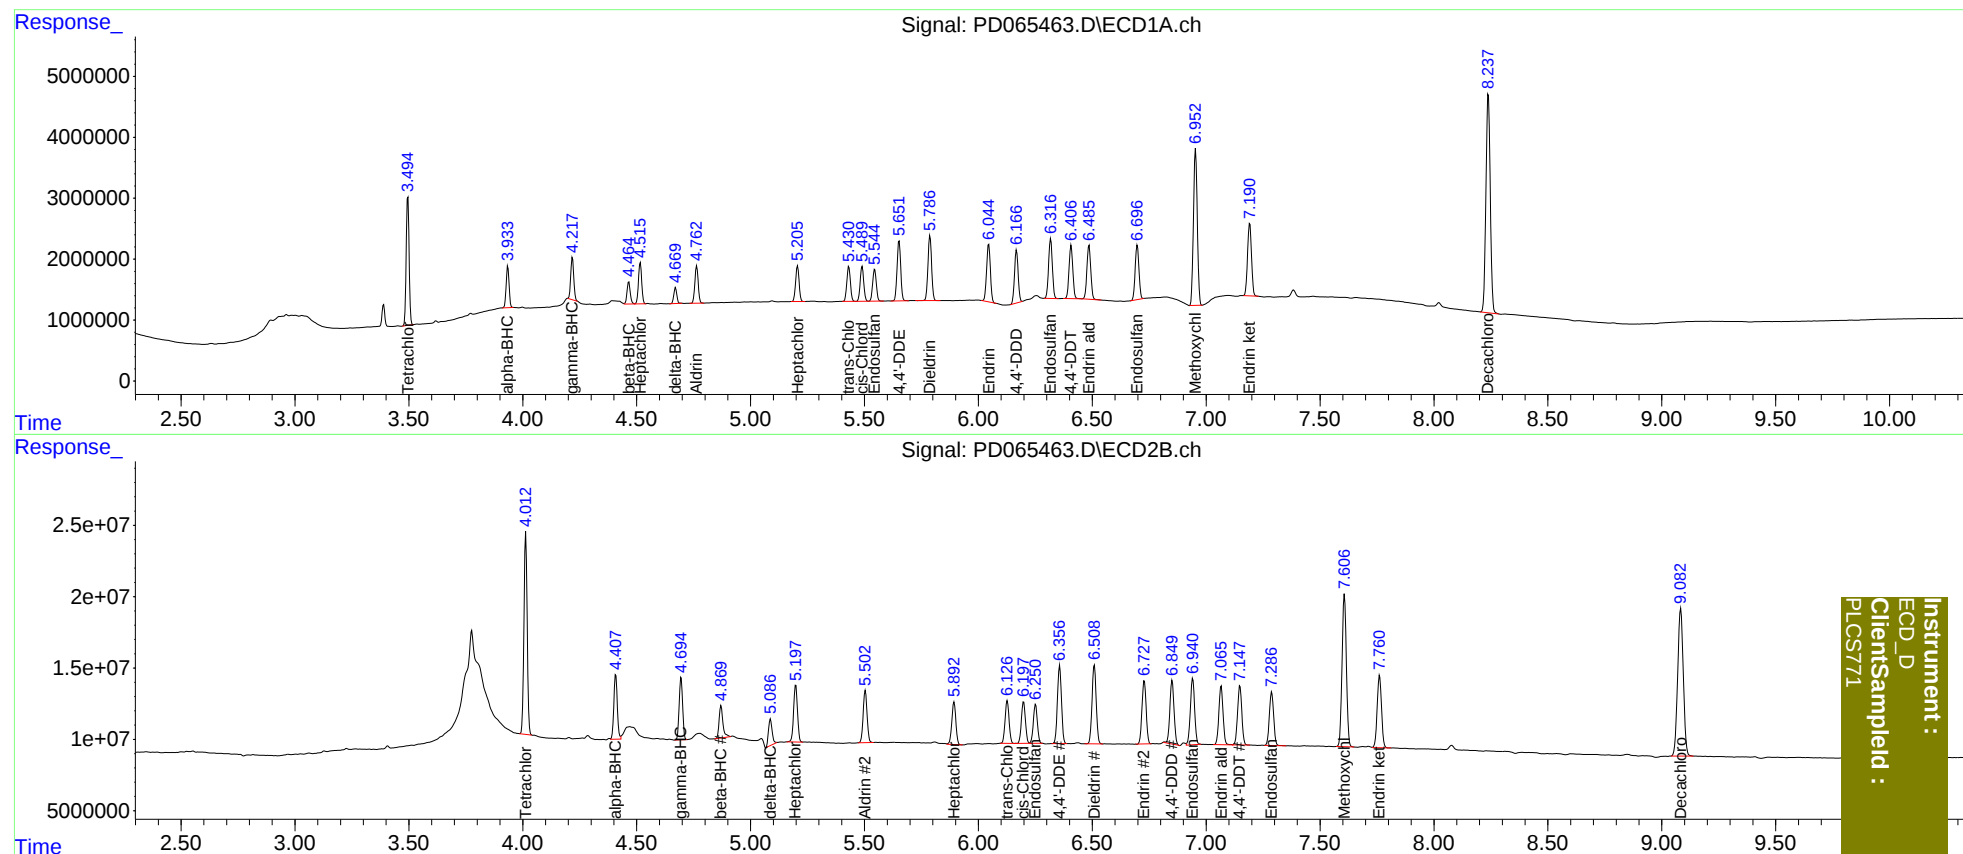

Instrument :
ECD_D
ClientSampled :
PLC5771