

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083024\
 Data File : PD084809.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2024 15:13
 Operator : AR\AJ
 Sample : P3721-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCXZ3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 09:01:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.906	10073197	38904215	9.960	10.994
27)	SA Decachlor...	9.036	8.109	10575121	43864330	8.097	12.615 #
Target Compounds							
5)	MB Aldrin	5.280f	0.000	3182514	0	1.990	N.D. #
8)	B Heptachlo...	5.660	4.897	5852053	8835089	3.924	2.086 #
10)	B trans-Chl...	5.913	0.000	2657245	0	1.884	N.D. #
12)	B 4,4'-DDE	6.212f	5.435	4448255	18669662	3.566	4.759 #
13)	MA Dieldrin	6.276f	0.000	3053319	0	2.070	N.D. #
16)	A 4,4'-DDD	0.000	5.895f	0	9571288	N.D.	2.820
20)	A Methoxychlor	7.419f	0.000	1070191	0	2.054	N.D. #
23)	Toxaphene-2	6.457f	5.435f	7502018	18669662	510.051	755.343 #
24)	Toxaphene-3	0.000	5.895	0	9571288	N.D.	405.626
26)	Toxaphene-5	7.896	0.000	8562995	0	454.531	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083024\
Data File : PD084809.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2024 15:13
Operator : AR\AJ
Sample : P3721-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 09:01:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

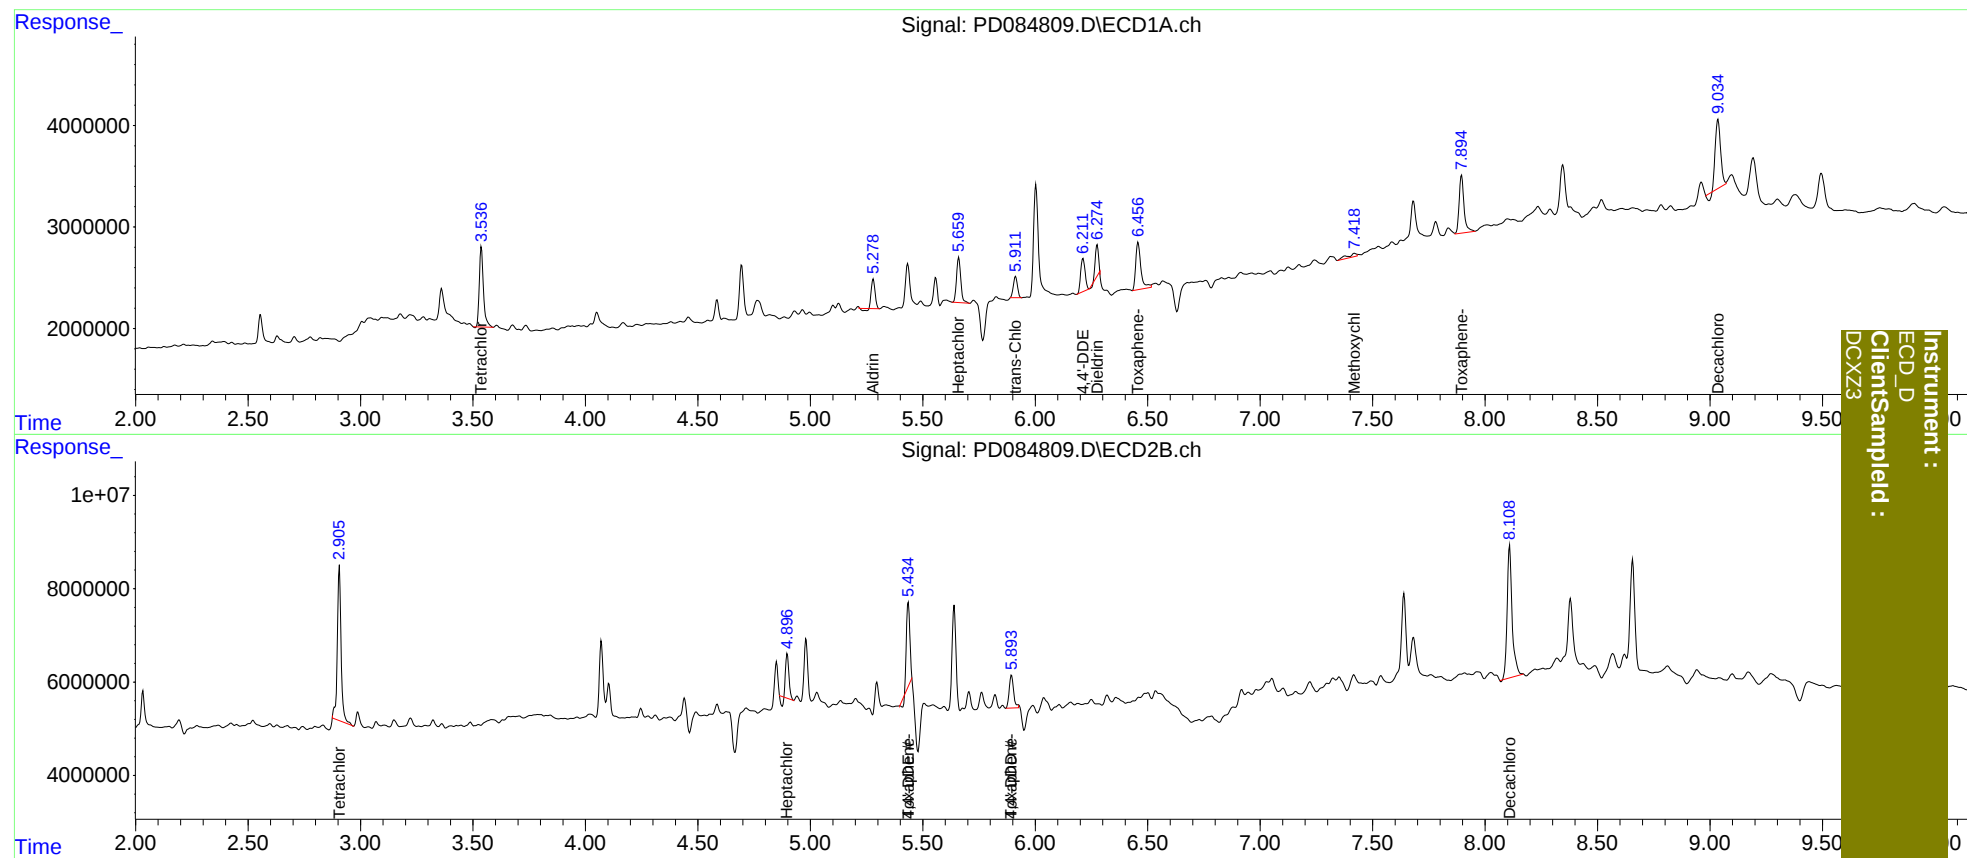


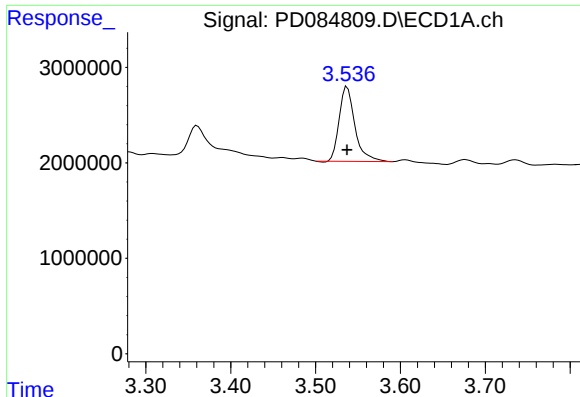

#1 Tetrachloro-m-xylene


R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 10073197
Conc: 9.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
DCXZ3

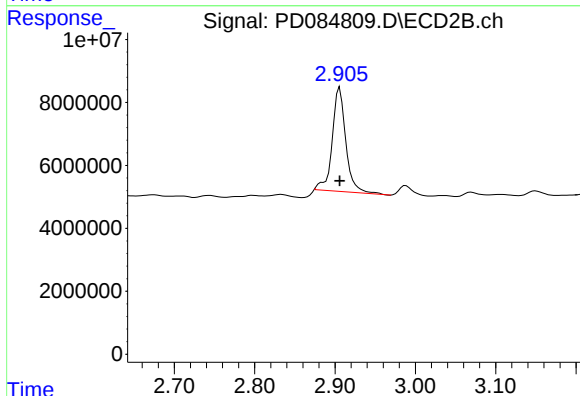


#1 Tetrachloro-m-xylene

R.T.: 2.906 min
Delta R.T.: 0.000 min
Response: 38904215
Conc: 10.99 ng/ml

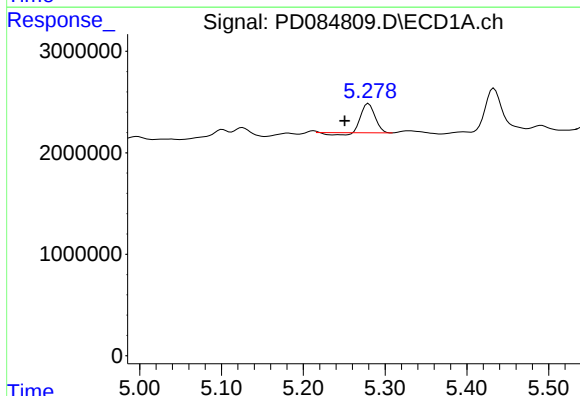


#5 Aldrin

R.T.: 5.280 min
Delta R.T.: 0.029 min
Response: 3182514
Conc: 1.99 ng/ml

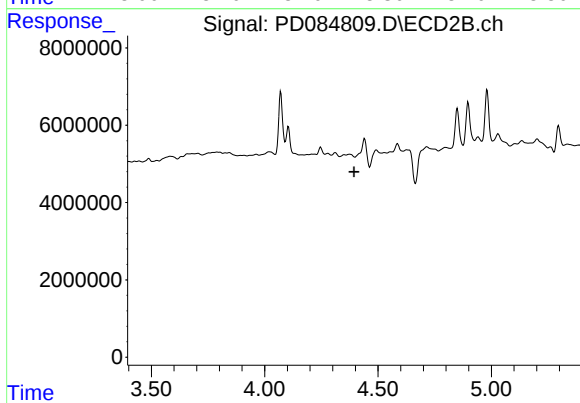

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 4.394 min
Response: 0
Conc: N.D.

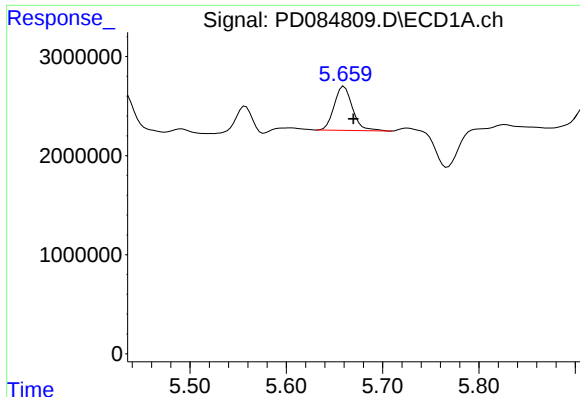

#8 Heptachlor epoxide


R.T.: 5.660 min
Delta R.T.: -0.009 min
Response: 5852053
Conc: 3.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
DCXZ3

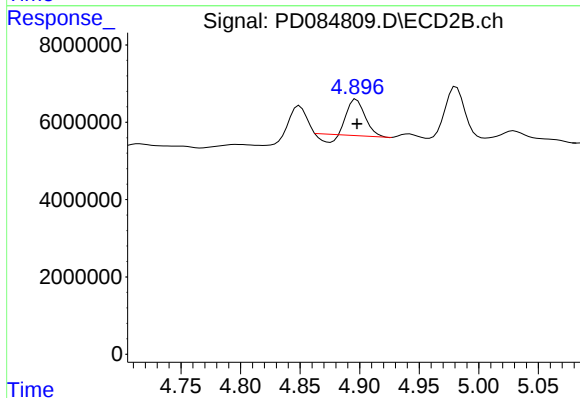


#8 Heptachlor epoxide

R.T.: 4.897 min
Delta R.T.: 0.000 min
Response: 8835089
Conc: 2.09 ng/ml

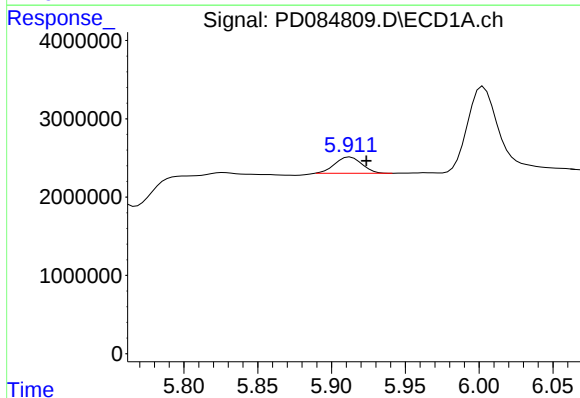


#10 trans-Chlordane

R.T.: 5.913 min
Delta R.T.: -0.011 min
Response: 2657245
Conc: 1.88 ng/ml

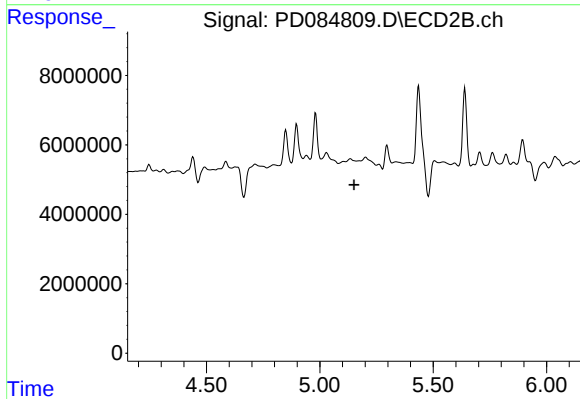

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.152 min
Response: 0
Conc: N.D.

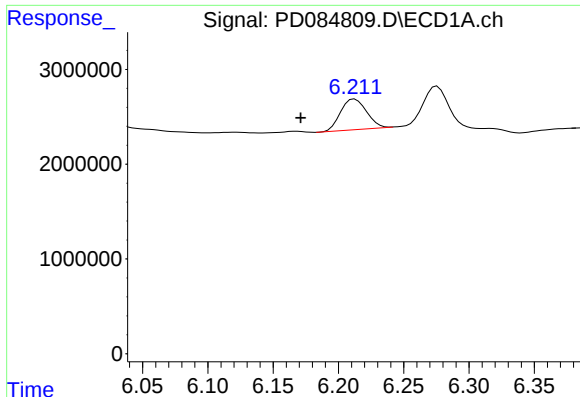

#12 4,4'-DDE


R.T.: 6.212 min
Delta R.T.: 0.041 min
Response: 4448255
Conc: 3.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
DCXZ3

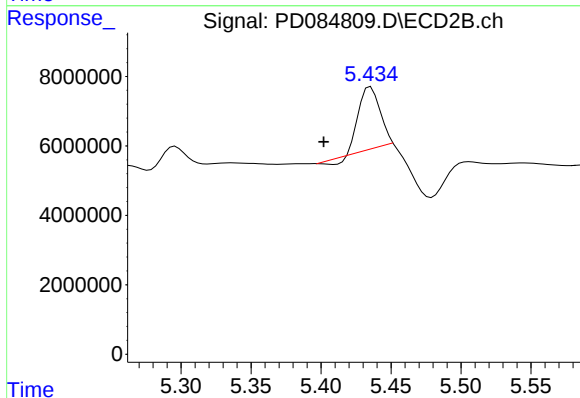


#12 4,4'-DDE

R.T.: 5.435 min
Delta R.T.: 0.034 min
Response: 18669662
Conc: 4.76 ng/ml

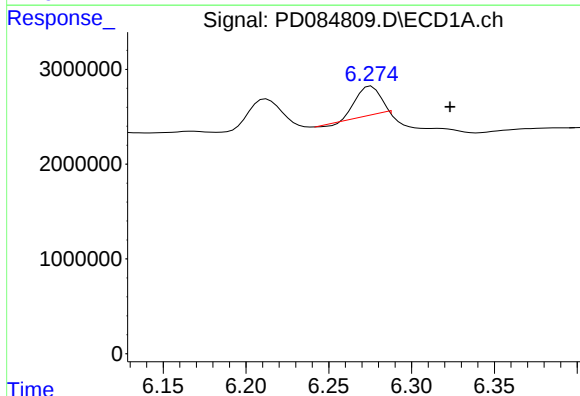


#13 Dieldrin

R.T.: 6.276 min
Delta R.T.: -0.048 min
Response: 3053319
Conc: 2.07 ng/ml

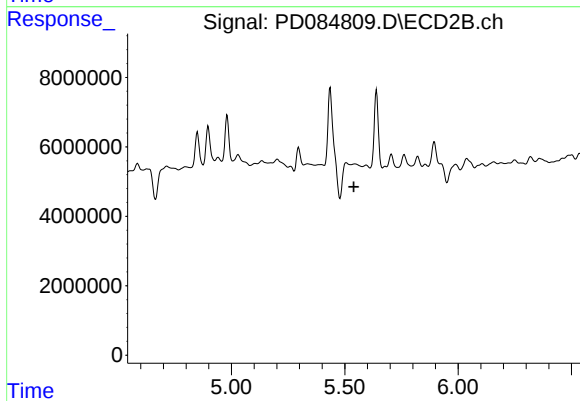

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 5.540 min
Response: 0
Conc: N.D.

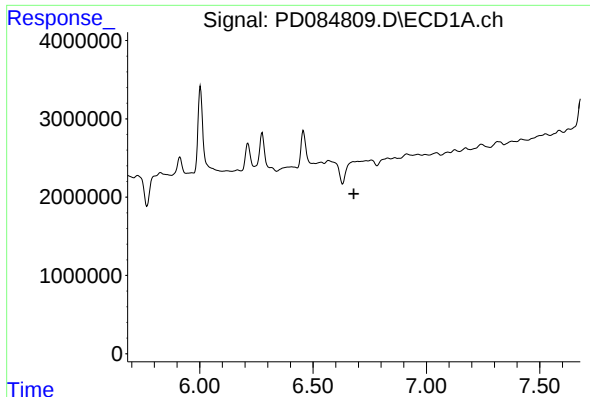

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DCXZ3

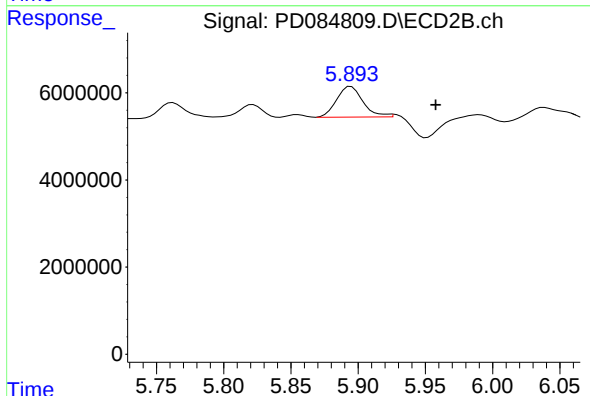


#16 4,4'-DDD

R.T.: 5.895 min
Delta R.T.: -0.063 min
Response: 9571288
Conc: 2.82 ng/ml

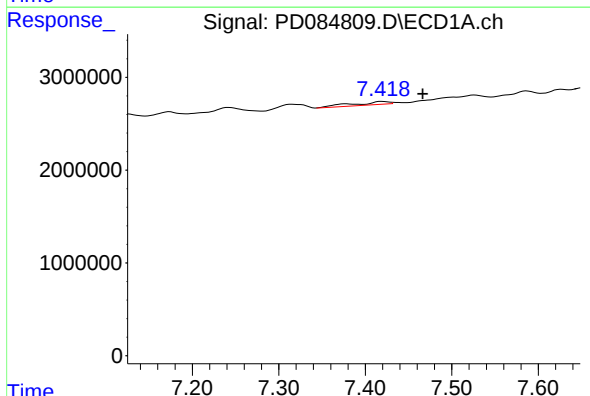


#20 Methoxychlor

R.T.: 7.419 min
Delta R.T.: -0.047 min
Response: 1070191
Conc: 2.05 ng/ml

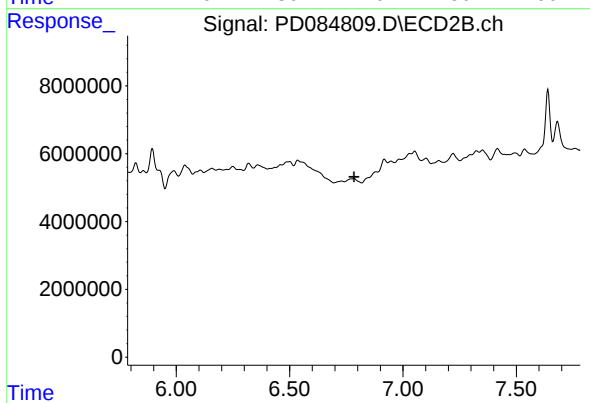

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.785 min
Response: 0
Conc: N.D.

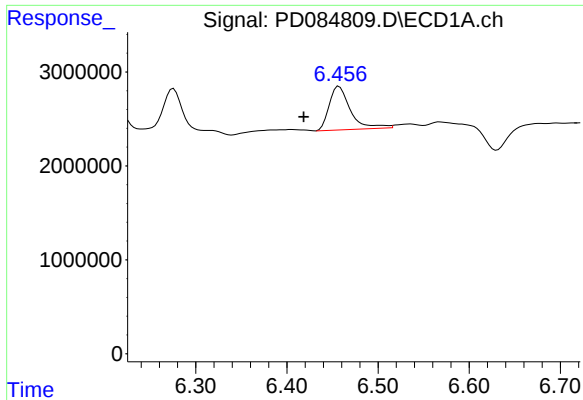

#23 Toxaphene-2


R.T.: 6.457 min
Delta R.T.: 0.039 min
Response: 7502018
Conc: 510.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
DCXZ3

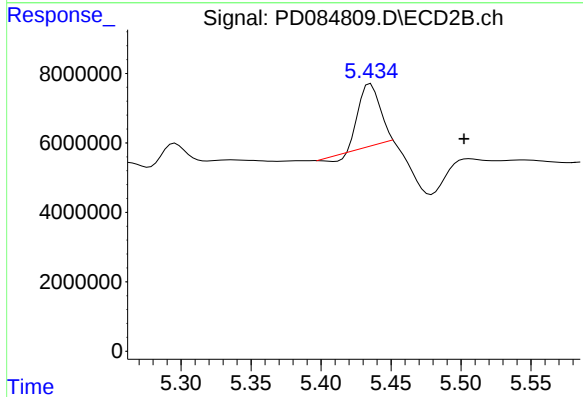


#23 Toxaphene-2

R.T.: 5.435 min
Delta R.T.: -0.067 min
Response: 18669662
Conc: 755.34 ng/ml

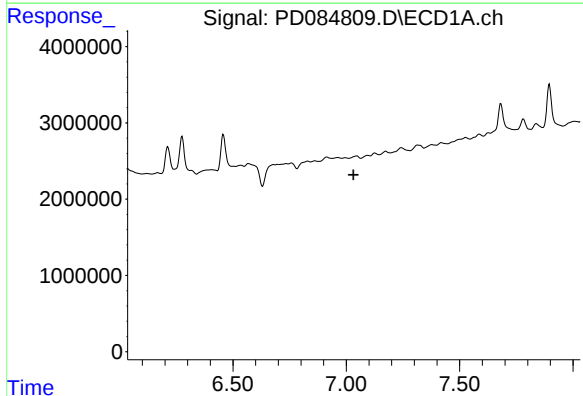


#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T. : 7.032 min
Response: 0
Conc: N.D.

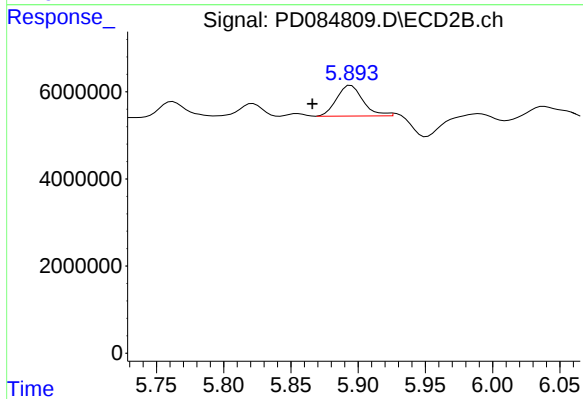

#24 Toxaphene-3


R.T.: 5.895 min
Delta R.T.: 0.029 min
Response: 9571288
Conc: 405.63 ng/ml

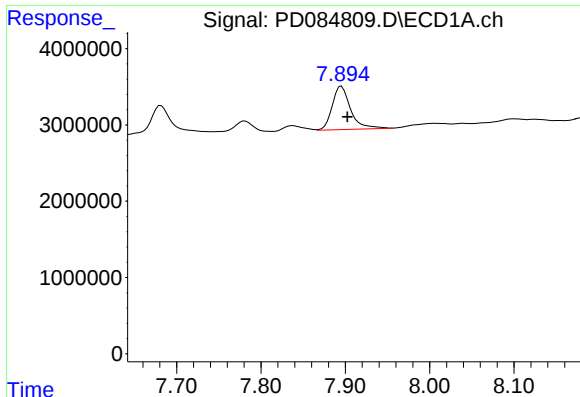

#26 Toxaphene-5


R.T.: 7.896 min
Delta R.T.: -0.007 min
Response: 8562995
Conc: 454.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
DCXZ3

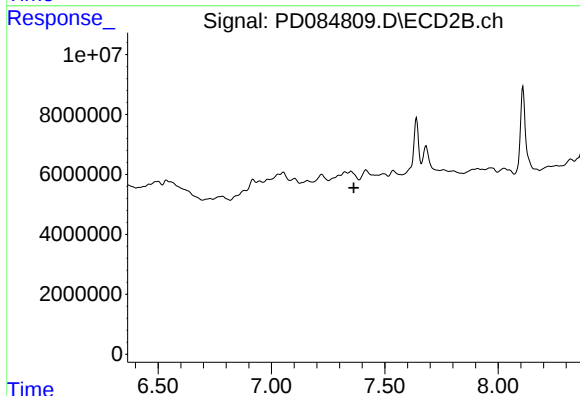


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T. : 7.363 min
Response: 0
Conc: N.D.

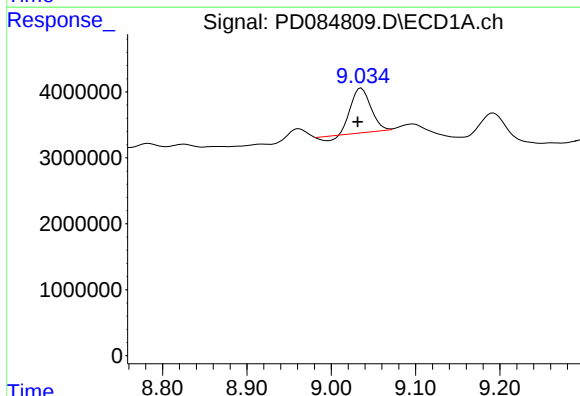

#27 Decachlorobiphenyl

R.T.: 9.036 min
Delta R.T.: 0.004 min
Response: 10575121
Conc: 8.10 ng/ml

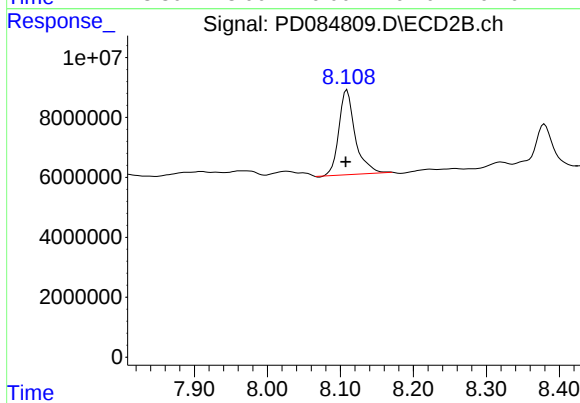

#27 Decachlorobiphenyl

R.T.: 8.109 min
Delta R.T.: 0.002 min
Response: 43864330
Conc: 12.61 ng/ml