

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083024\
 Data File : PD084797.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2024 11:47
 Operator : AR\AJ
 Sample : P3675-20MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCYA1MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/29/2024
 Supervised By :Ankita Jodhani 08/29/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 03:27:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.553	2.905	12666124	46768573	12.523	13.216
2)	SA Decachlor...	9.048	8.107	15088953	35552212	11.553	10.224
Target Compounds							
2)	A alpha-BHC	3.999	3.417	103.2E6	282.0E6	60.708	55.621
3)	MA gamma-BHC...	4.328	3.752	99396669	269.6E6	61.437	55.640
4)	MA Heptachlor	4.925	4.106	94140240	239.3E6	61.186m	56.216
5)	MB Aldrin	5.267	4.391	92306923	237.1E6	57.715	53.391m
6)	B beta-BHC	4.511	4.043	39042974	112.9E6	53.751	52.096m
7)	B delta-BHC	4.759	4.283	94710955	270.6E6	57.750	54.507
8)	B Heptachlo...	5.684	4.897	90293996	225.1E6	60.540m	53.144
9)	A Endosulfan I	6.067	5.271	76678364	184.3E6	55.734m	48.082m
10)	B trans-Chl...	5.939	5.151	79863832	223.6E6	56.626	54.361
11)	B cis-Chlor...	6.020	5.216	82794249	222.2E6	55.997m	52.956
12)	B 4,4'-DDE	6.189	5.401	151.1E6	429.5E6	121.090	109.495
13)	MA Dieldrin	6.339	5.540	171.1E6	457.5E6	116.014m	106.488
14)	MA Endrin	6.566	5.817	147.3E6	433.2E6	130.512m	117.009
15)	B Endosulfa...	6.777	6.108	142.9E6	402.0E6	108.244m	108.415m
16)	A 4,4'-DDD	6.696	5.958	126.8E6	378.8E6	128.391m	111.628
17)	MA 4,4'-DDT	7.012	6.213	108.1E6	335.9E6	120.731m	104.992
18)	B Endrin al...	6.905	6.288	105.3E6	303.8E6	116.601m	106.418
19)	B Endosulfa...	7.140	6.512	135.3E6	381.8E6	117.426	106.900
20)	A Methoxychlor	7.482	6.785	306.5E6	826.5E6	588.484m	499.636
21)	B Endrin ke...	7.619	7.023	144.9E6	441.9E6	118.527m	100.362

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083024\
Data File : PD084797.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2024 11:47
Operator : AR\AJ
Sample : P3675-20MS
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 03:27:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

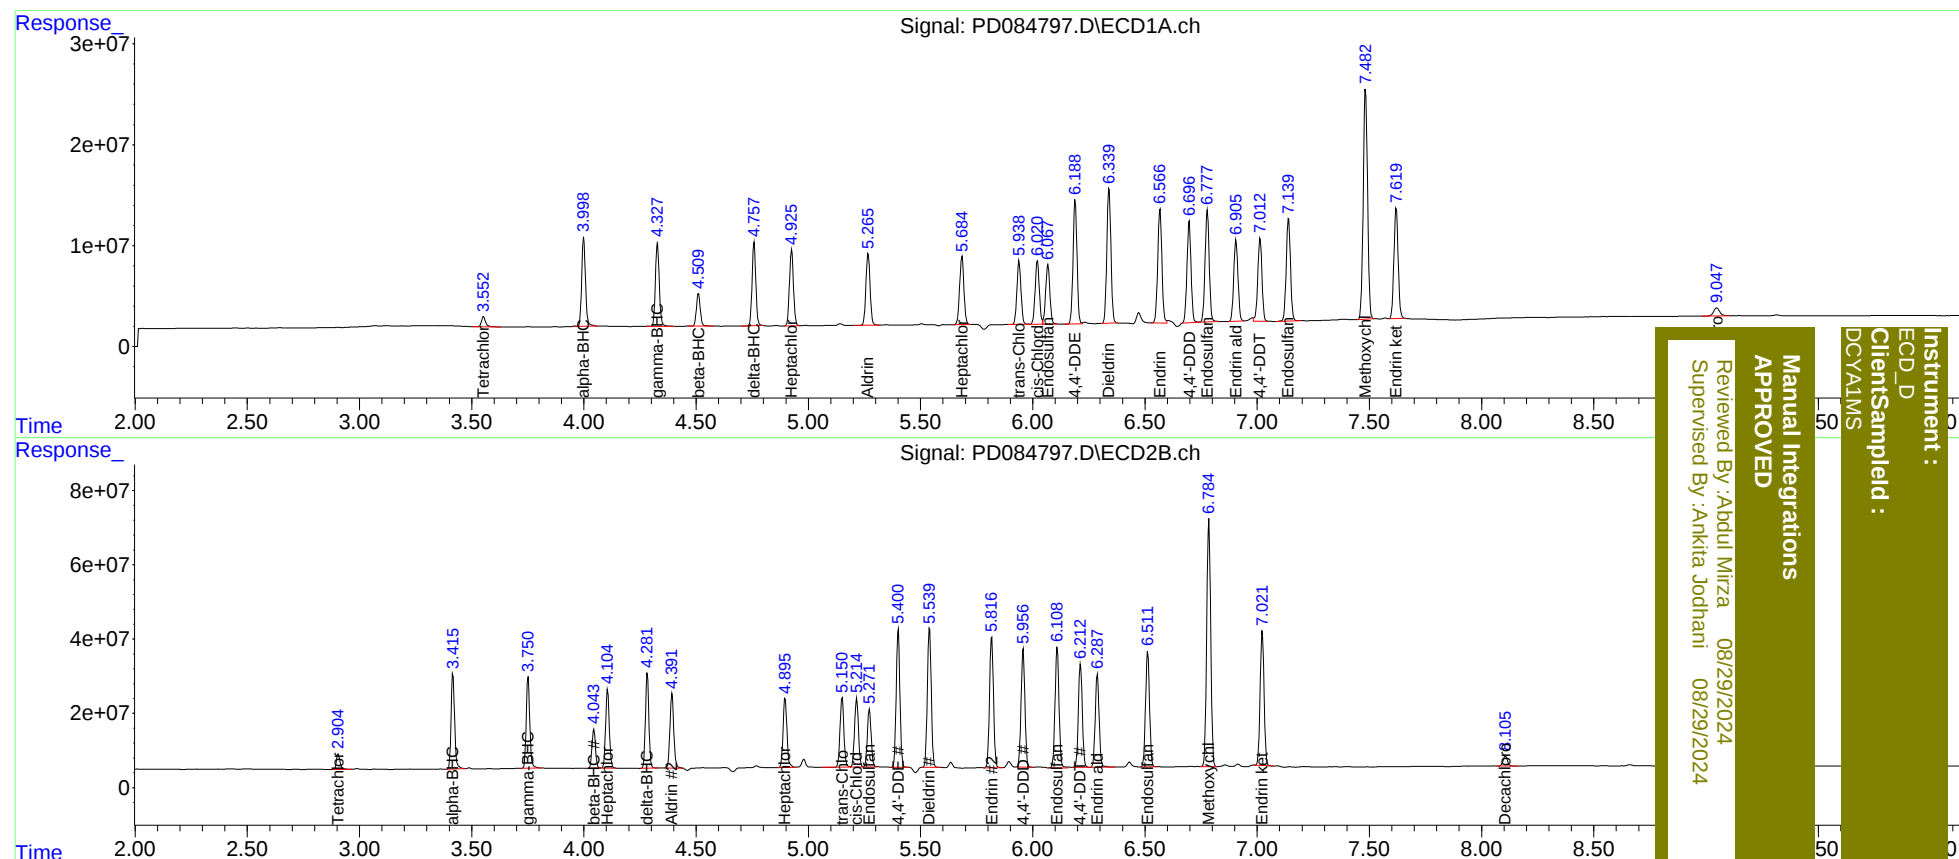

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 08/29/2024
Supervised By: Ankita Jodhani 08/29/2024

Instrument :
ECD_D
Client Sampled :
DCYALMS