

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083024\
 Data File : PD084801.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Aug 2024 12:41
 Operator : AR\AJ
 Sample : PP23634
 Misc : PEST/SPIK9(SFAM)500/1000 10X
 ALS Vial : 100 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PP23634

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/29/2024
 Supervised By :Ankita Jodhani 08/29/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 29 03:28:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds


2) A	alpha-BHC	3.982	3.417	85013065	230.8E6	50.003	45.526
3) MA	gamma-BHC...	4.312	3.752	80883161	222.2E6	49.994	45.864
4) MA	Heptachlor	4.909	4.107	78524268	195.0E6	51.036	45.818
5) MB	Aldrin	5.250	4.393	79031073	202.5E6	49.414	45.592
6) B	beta-BHC	4.494	4.045	32271923	92932866	44.429	42.867
7) B	delta-BHC	4.741	4.283	78050825	224.0E6	47.592	45.124
8) B	Heptachlo...	5.669	4.897	69134788	186.7E6	46.354	44.079
9) A	Endosulfan I	6.050	5.271	65271505	178.1E6	47.443m	46.466m
10) B	trans-Chl...	5.922	5.151	68292373	187.3E6	48.421	45.545
11) B	cis-Chlor...	6.002	5.216	69018281	184.1E6	46.679m	43.876
12) B	4,4'-DDE	6.172	5.401	129.1E6	361.4E6	103.526	92.134
13) MA	Dieldrin	6.324	5.540	144.5E6	387.7E6	97.988	90.246
14) MA	Endrin	6.549	5.818	123.6E6	360.8E6	109.520m	97.441
15) B	Endosulfa...	6.760	6.109	122.2E6	331.9E6	92.536	89.522
16) A	4,4'-DDD	6.680	5.957	109.3E6	349.3E6	110.666	102.938m
17) MA	4,4'-DDT	6.995	6.213	81086407	255.7E6	90.586m	79.942
18) B	Endrin al...	6.889	6.288	90343527	260.8E6	100.037	91.346
19) B	Endosulfa...	7.123	6.512	113.6E6	326.3E6	98.646	91.349
20) A	Methoxychlor	7.466	6.785	227.0E6	666.4E6	435.690	402.862
21) B	Endrin ke...	7.602	7.023	118.0E6	374.5E6	96.525	85.043

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083024\
Data File : PD084801.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Aug 2024 12:41
Operator : AR\AJ
Sample : PP23634
Misc : PEST/SPIK9(SFAM)500/1000 10X
ALS Vial : 100 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 29 03:28:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

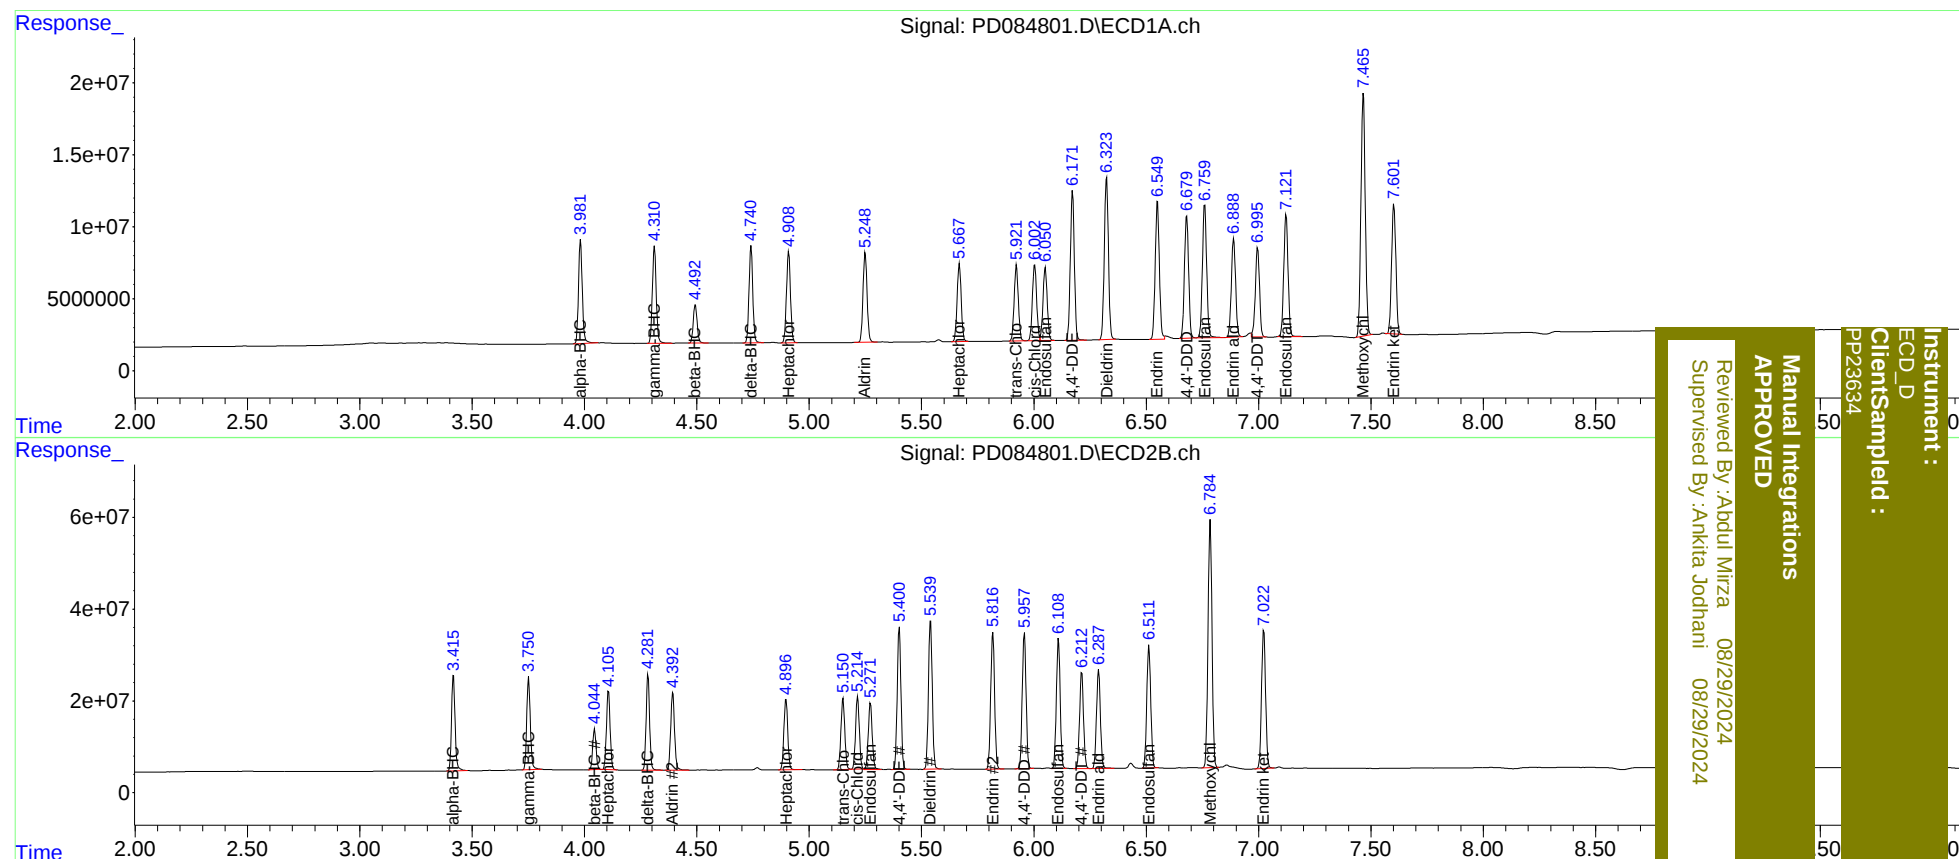

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 08/29/2024
Supervised By: Ankita Jodhani 08/29/2024

Instrument :
ECD_D
Client Sampled :
PP23634