

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083123\
 Data File : PD077488.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2023 18:52
 Operator : AR\AJ
 Sample : 04166-08
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 21:34:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:53:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.761	53459923	32008212	24.351	25.694
27)	SA Decachlor...	9.084	7.902	99186891	56428966	38.979	45.269
Target Compounds							
3)	MA gamma-BHC...	4.326	0.000	3152762	0	0.924	N.D. #
4)	MA Heptachlor	0.000	3.942	0	1277133	N.D.	0.741
6)	B beta-BHC	0.000	3.846f	0	513575	N.D.	0.629
15)	B Endosulfa...	6.781	5.877f	1451225	117519	0.514	<MDL #
16)	A 4,4'-DDD	6.781f	0.000	1451225	0	0.668	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083123\
Data File : PD077488.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2023 18:52
Operator : AR\AJ
Sample : 04166-08
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 21:34:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 01:53:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

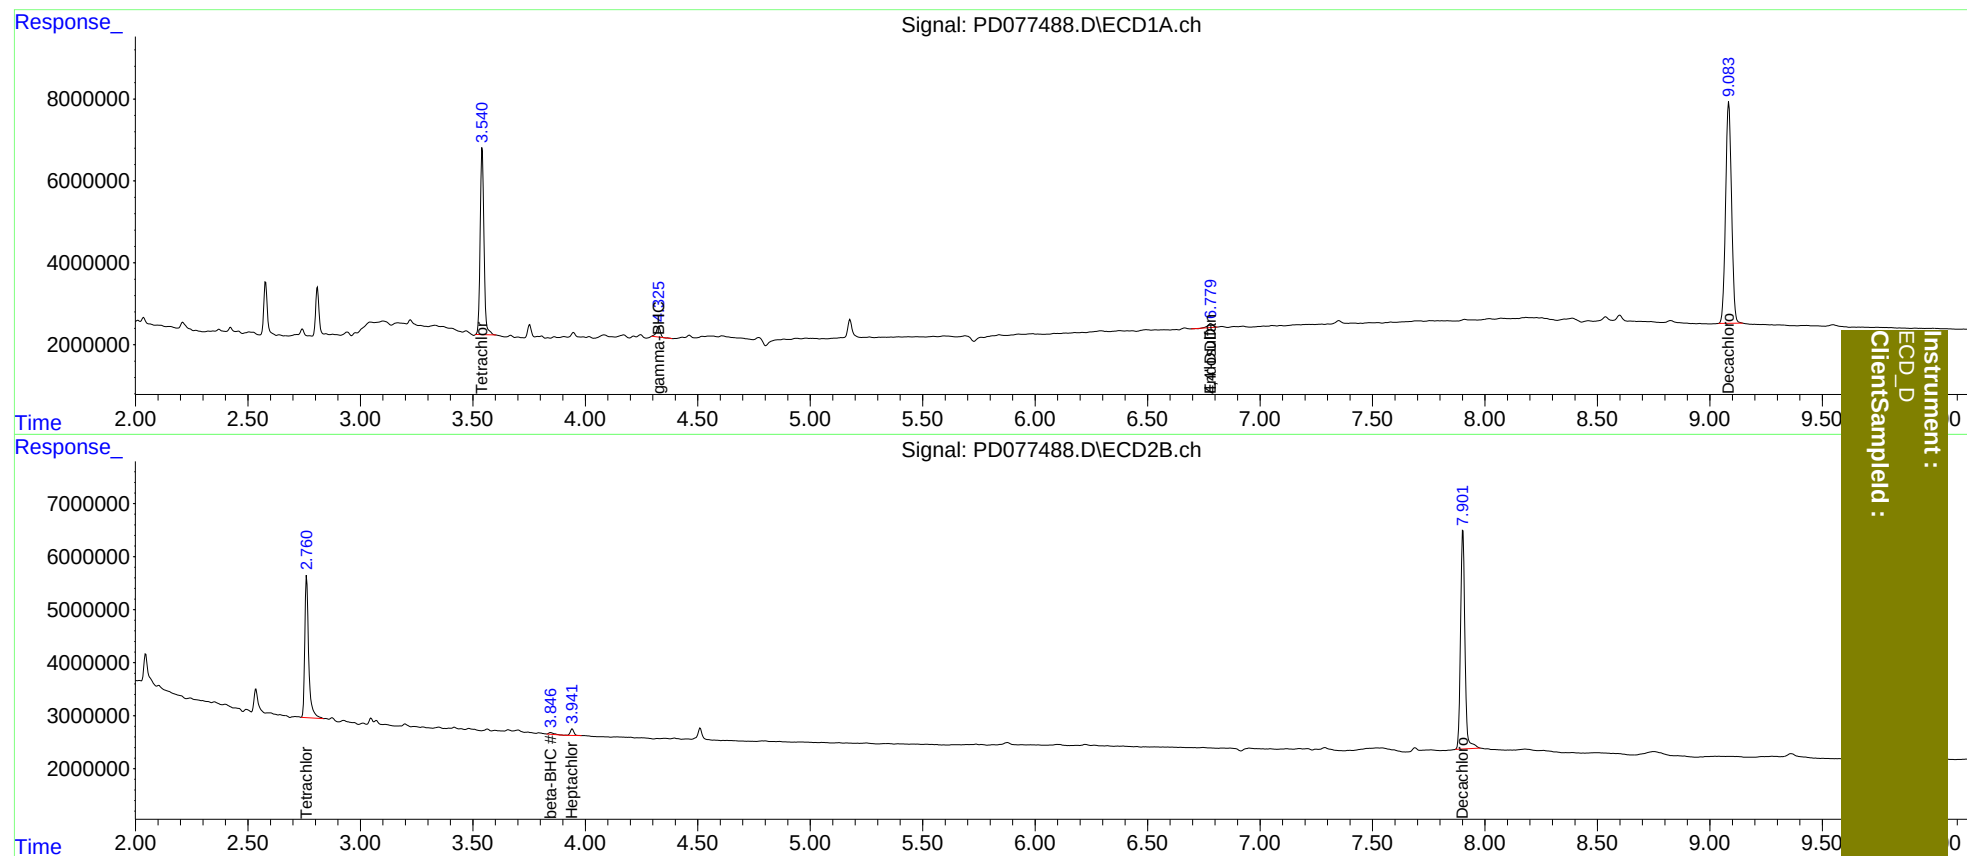


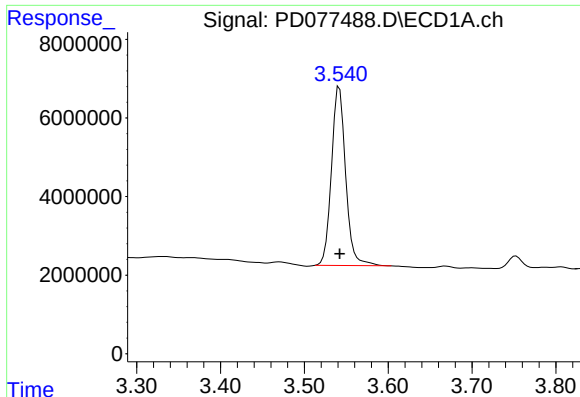

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.000 min
Response: 53459923
Conc: 24.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

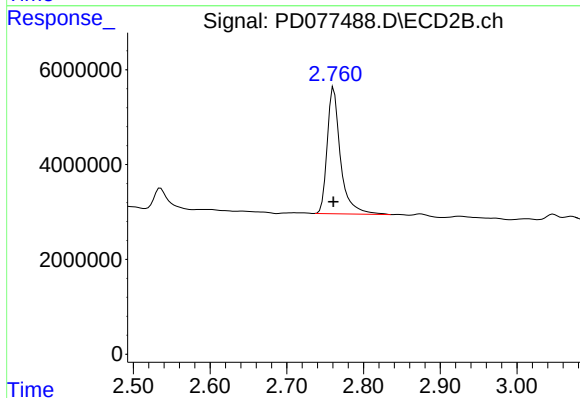


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: 0.000 min
Response: 32008212
Conc: 25.69 ng/ml

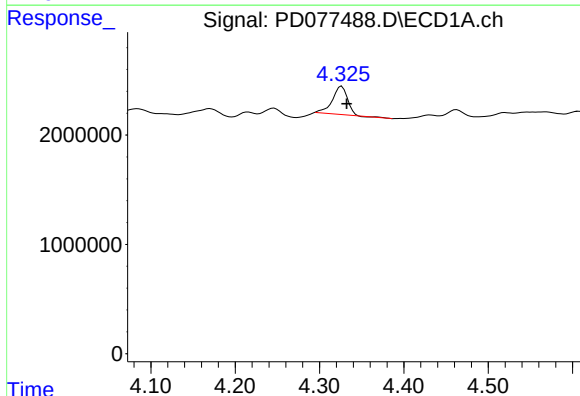


#3 gamma-BHC (Lindane)

R.T.: 4.326 min
Delta R.T.: -0.006 min
Response: 3152762
Conc: 0.92 ng/ml

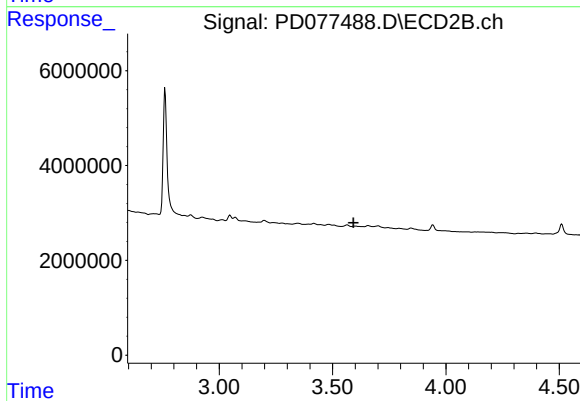

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 3.592 min
Response: 0
Conc: N.D.

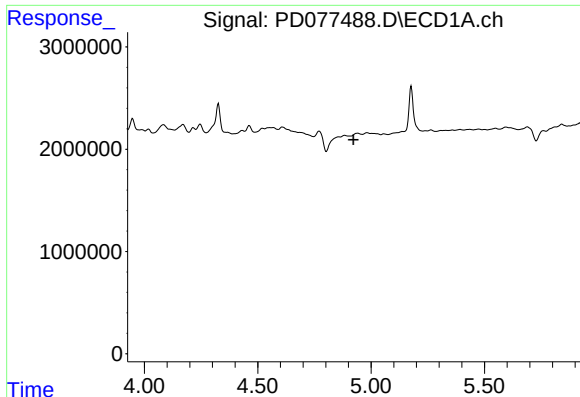

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.923 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

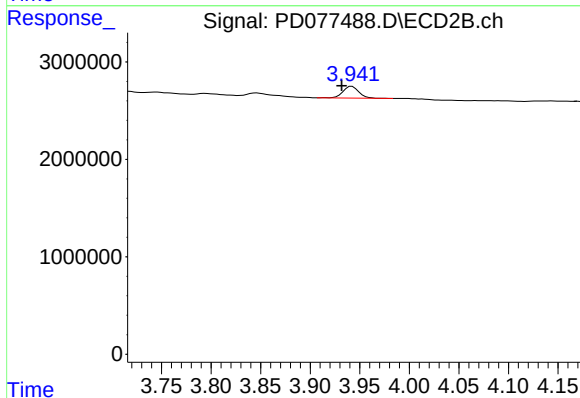


#4 Heptachlor

R.T.: 3.942 min
Delta R.T.: 0.010 min
Response: 1277133
Conc: 0.74 ng/ml

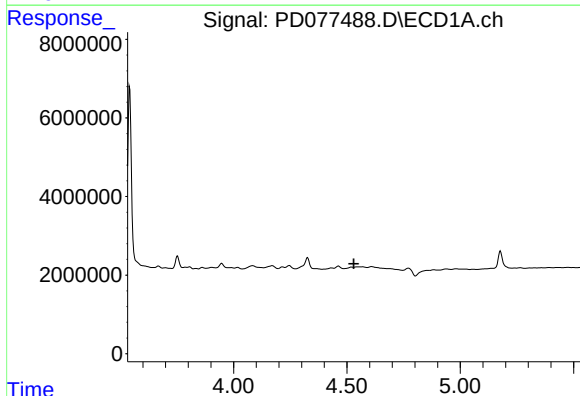


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.530 min
Response: 0
Conc: N.D.

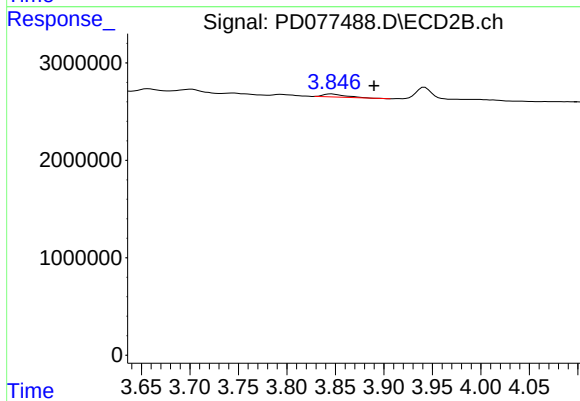

#6 beta-BHC


R.T.: 3.846 min
Delta R.T.: -0.044 min
Response: 513575
Conc: 0.63 ng/ml

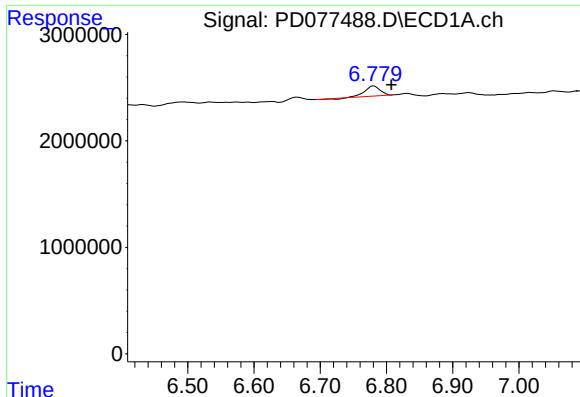

#15 Endosulfan II


R.T.: 6.781 min
Delta R.T.: -0.027 min
Response: 1451225
Conc: 0.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

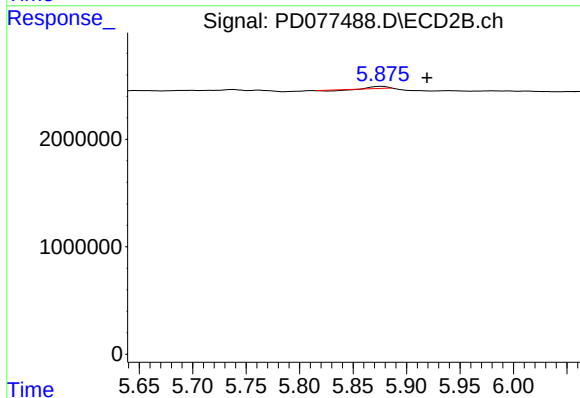


#15 Endosulfan II

R.T.: 5.877 min
Delta R.T.: -0.042 min
Response: 117519
Conc: N.D.

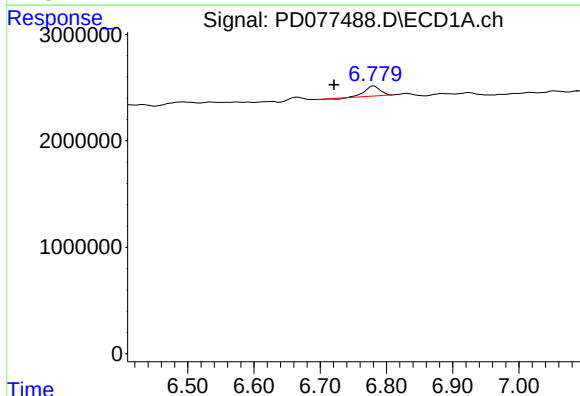


#16 4,4'-DDD

R.T.: 6.781 min
Delta R.T.: 0.060 min
Response: 1451225
Conc: 0.67 ng/ml

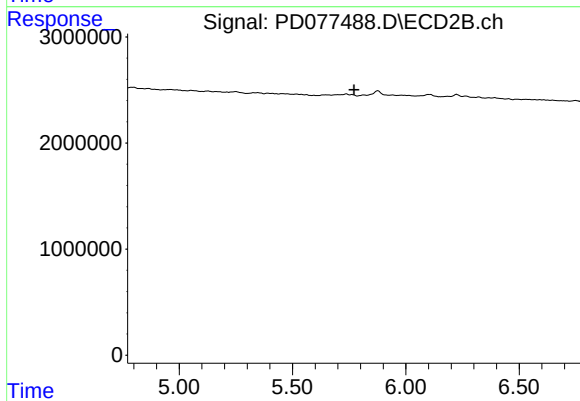

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.772 min
Response: 0
Conc: N.D.

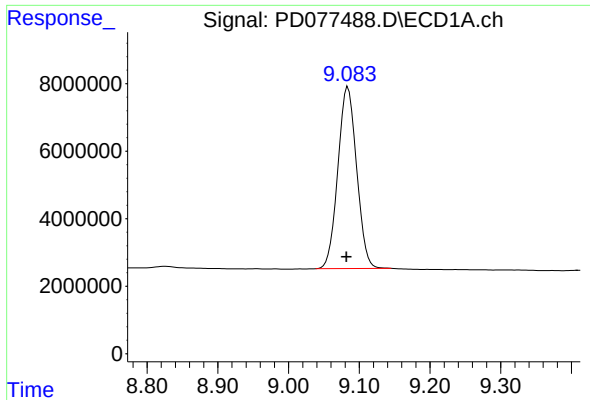

#27 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.002 min
Response: 99186891
Conc: 38.98 ng/ml

Instrument :
ECD_D
ClientSampleId :

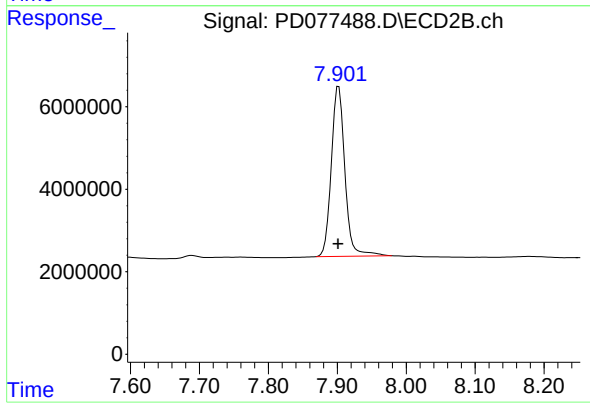

#27 Decachlorobiphenyl

R.T.: 7.902 min
Delta R.T.: 0.000 min
Response: 56428966
Conc: 45.27 ng/ml