

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083123\
 Data File : PD077506.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2023 23:19
 Operator : AR\AJ
 Sample : 04153-08
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 00:36:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:53:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.761	46023206	26973334	20.964	21.652
27)	SA Decachlor...	9.084	7.902	66560453	35451056	26.157	28.440
Target Compounds							
2)	A alpha-BHC	3.949f	0.000	1214584	0	0.336	N.D. #
3)	MA gamma-BHC...	0.000	3.600	0	93413	N.D.	<MDL
6)	B beta-BHC	0.000	3.845f	0	392454	N.D.	0.481
15)	B Endosulfa...	0.000	5.877f	0	208381	N.D.	0.156

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083123\
Data File : PD077506.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2023 23:19
Operator : AR\AJ
Sample : 04153-08
Misc :
ALS Vial : 39 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 00:36:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 01:53:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

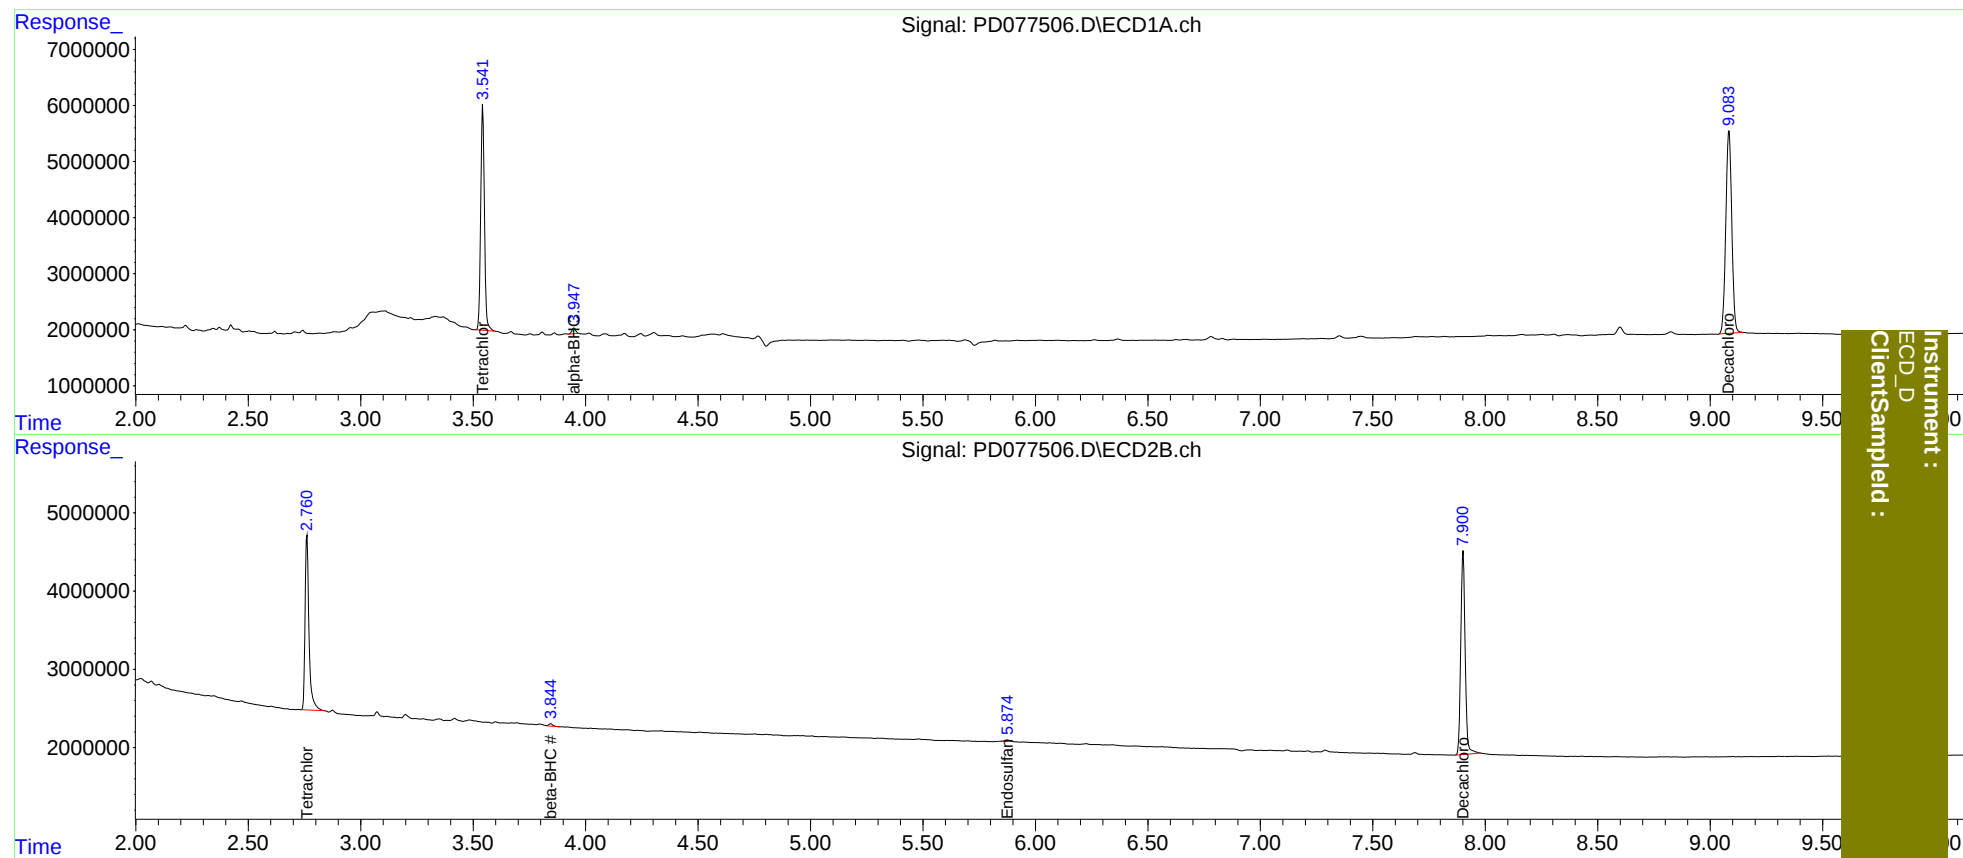


Instrument :
ECD_D
ClientSampled :
0

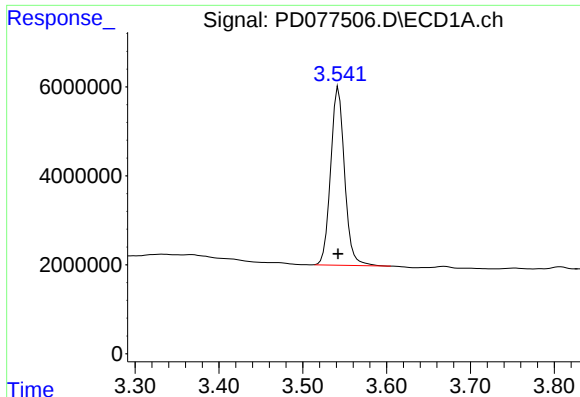

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 46023206
Conc: 20.96 ng/ml

Instrument :
ECD_D
ClientSampleId :

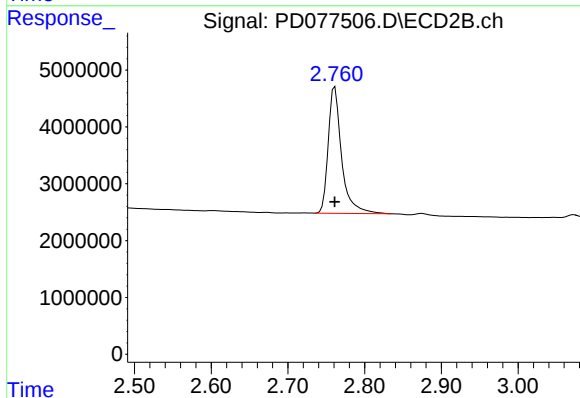


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: 0.000 min
Response: 26973334
Conc: 21.65 ng/ml

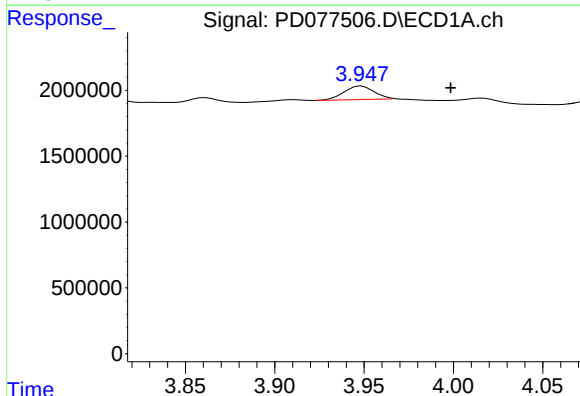


#2 alpha-BHC

R.T.: 3.949 min
Delta R.T.: -0.050 min
Response: 1214584
Conc: 0.34 ng/ml

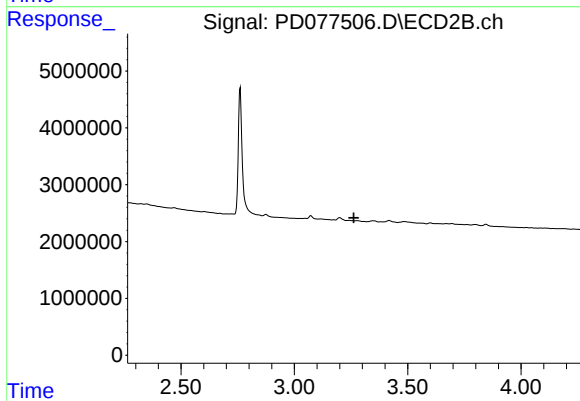

#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.263 min
Response: 0
Conc: N.D.

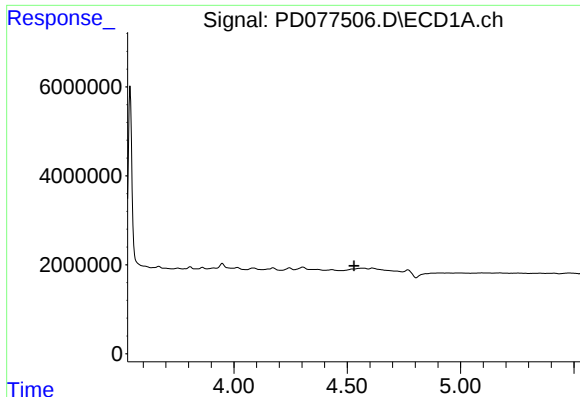

#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.530 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

#6 beta-BHC


R.T.: 3.845 min
Delta R.T.: -0.045 min
Response: 392454
Conc: 0.48 ng/ml

#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.808 min
Response: 0
Conc: N.D.

#15 Endosulfan II


R.T.: 5.877 min
Delta R.T.: -0.043 min
Response: 208381
Conc: 0.16 ng/ml

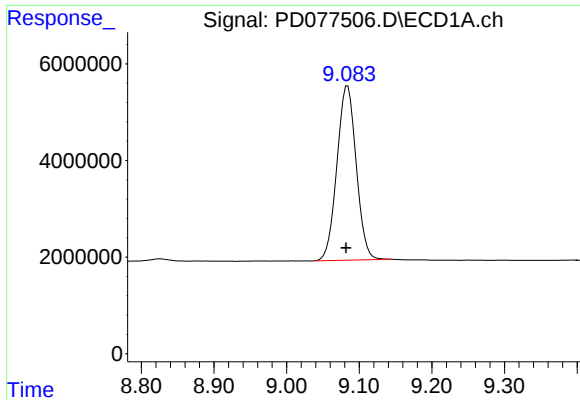

#27 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.002 min
Response: 66560453
Conc: 26.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

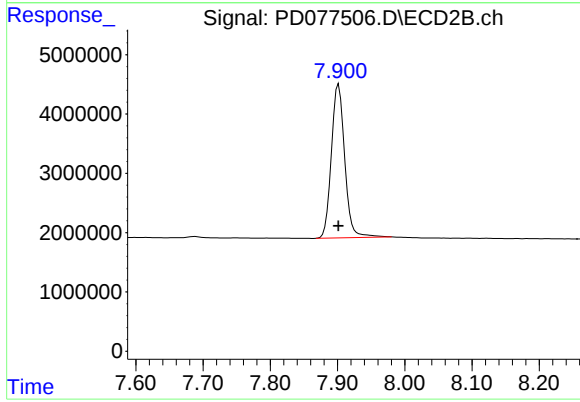

#27 Decachlorobiphenyl

R.T.: 7.902 min
Delta R.T.: 0.000 min
Response: 35451056
Conc: 28.44 ng/ml