

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083123\
 Data File : PD077472.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2023 12:27
 Operator : AR\AJ
 Sample : 04123-08MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH9Q4MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/31/2023
 Supervised By : Ankita Jodhani 08/31/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 21:27:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:53:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.762	45774646	25675462	20.850	20.610
27)	SA Decachlor...	9.086	7.902	61777024	30210108	24.278	24.235
Target Compounds							
2)	A alpha-BHC	4.000	3.262	206.7E6	105.8E6	57.212	57.550m
3)	MA gamma-BHC...	4.334	3.593	190.0E6	97357528	55.660	56.450
4)	MA Heptachlor	4.925	3.932	183.0E6	93836242	52.311	54.450
5)	MB Aldrin	5.268	4.211	183.1E6	87549772	52.855	50.590m
6)	B beta-BHC	4.531	3.890	77560124	40154276	49.978	49.187
7)	B delta-BHC	4.779	4.120	189.1E6	97708612	57.051	56.257
8)	B Heptachlo...	5.695	4.714	166.8E6	86122099	52.268	52.645
9)	A Endosulfan I	6.082	5.084	157.5E6	75373582	55.728	53.496
10)	B trans-Chl...	5.952	4.965	162.8E6	82855543	52.699	53.648
11)	B cis-Chlor...	6.031	5.029	164.9E6	83145628	51.505	51.627
12)	B 4,4'-DDE	6.203	5.217	318.2E6	157.3E6	111.087	115.562
13)	MA Dieldrin	6.358	5.349	355.0E6	180.9E6	113.891	114.025
14)	MA Endrin	6.589	5.625	284.5E6	153.8E6	111.913	110.772
15)	B Endosulfa...	6.809	5.919	294.6E6	152.4E6	104.235	113.918
16)	A 4,4'-DDD	6.723	5.772	258.4E6	127.6E6	118.881	128.339
17)	MA 4,4'-DDT	7.038	6.023	266.6E6	128.5E6	120.841	124.093
18)	B Endrin al...	6.939	6.099	213.0E6	110.5E6	98.938	101.691
19)	B Endosulfa...	7.174	6.321	245.7E6	137.8E6	98.720	110.049
20)	A Methoxychlor	7.513	6.598	690.7E6	324.3E6	536.899	574.895
21)	B Endrin ke...	7.660	6.828	319.1E6	170.3E6	113.379	115.664

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083123\
Data File : PD077472.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2023 12:27
Operator : AR\AJ
Sample : 04123-08MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 21:27:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 01:53:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

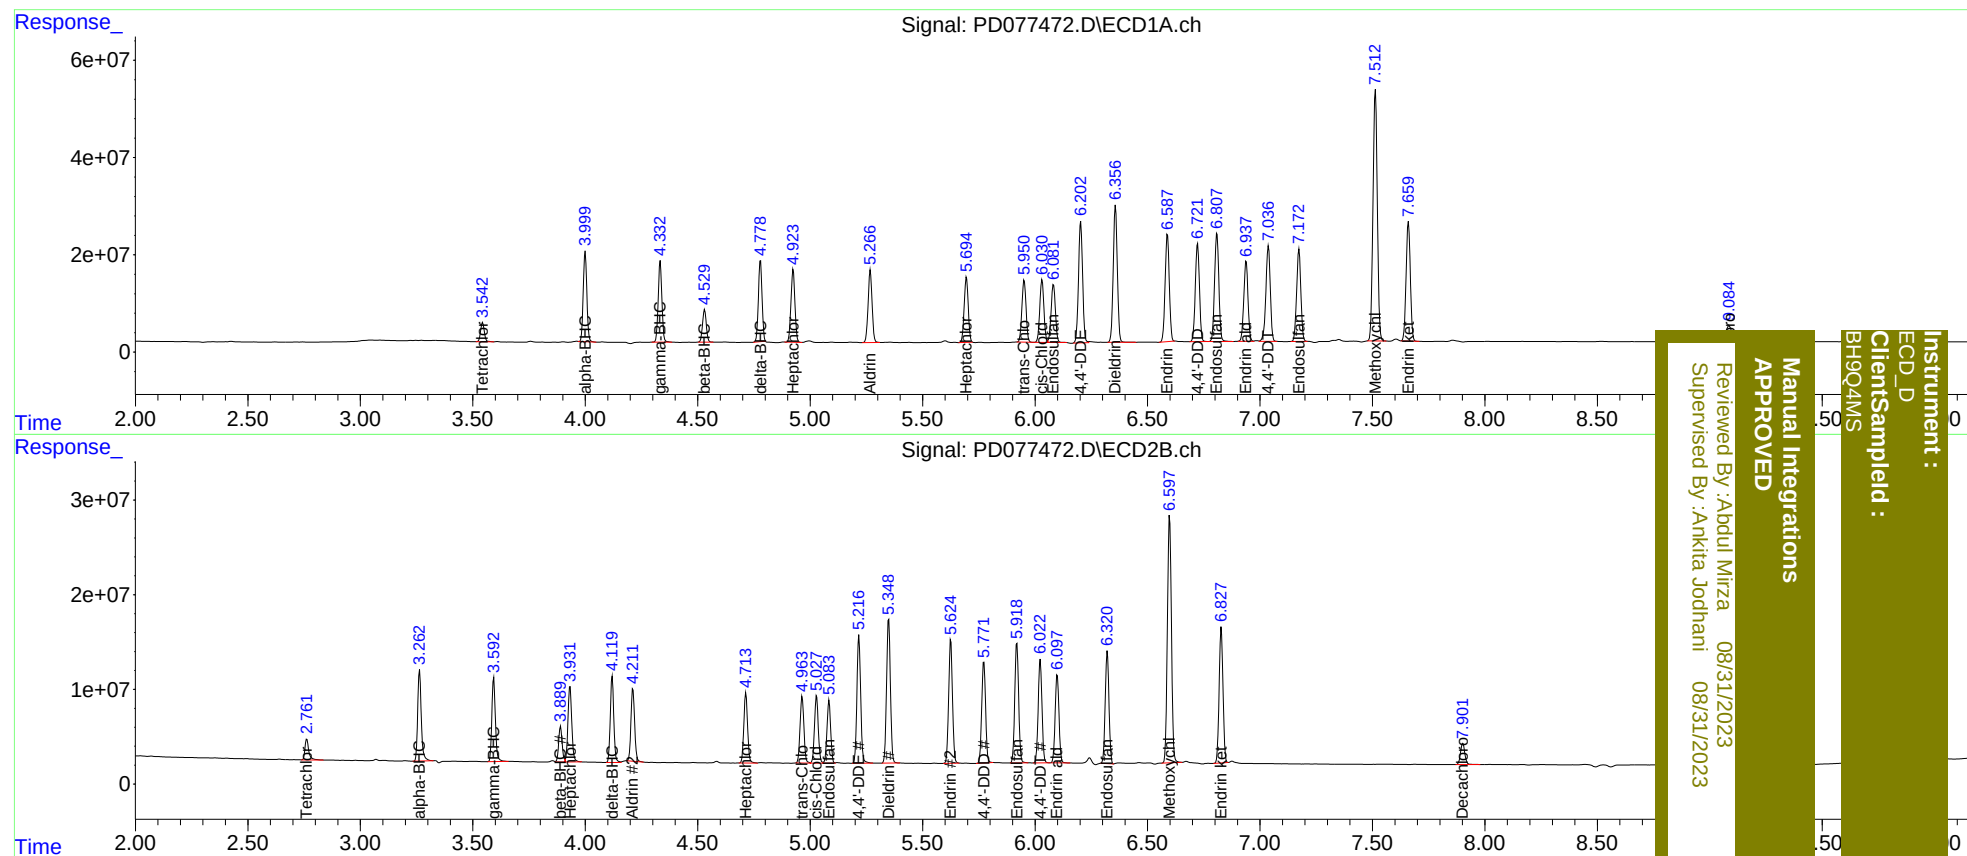

Instrument :
ECD_D
ClientSampled :
BH9Q4MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 08/31/2023
Supervised By: Ankita Jodhani 08/31/2023