

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083123\
 Data File : PD077473.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2023 12:41
 Operator : AR\AJ
 Sample : 04123-09MSD
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH9Q4MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/01/2023
 Supervised By : mohammad ahmed 09/01/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 21:28:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:53:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.763	45327214	25417797	20.647	20.404
27)	SA Decachlor...	9.086	7.902	61661634	30202890	24.232	24.230
Target Compounds							
2)	A alpha-BHC	4.001	3.262	204.9E6	105.7E6	56.704	57.487m
3)	MA gamma-BHC...	4.334	3.593	188.8E6	96920352	55.310	56.197
4)	MA Heptachlor	4.925	3.932	182.7E6	93628614	52.223	54.330
5)	MB Aldrin	5.268	4.211	182.6E6	87392320	52.717	50.499m
6)	B beta-BHC	4.532	3.890	77295837	39869310	49.808	48.838
7)	B delta-BHC	4.780	4.120	187.8E6	97321296	56.657	56.034
8)	B Heptachlo...	5.695	4.714	167.1E6	85689443	52.380	52.381
9)	A Endosulfan I	6.083	5.085	158.0E6	74658255	55.898	52.989
10)	B trans-Chl...	5.952	4.965	162.8E6	82698902	52.710	53.546
11)	B cis-Chlor...	6.031	5.029	165.2E6	82670688	51.582	51.332
12)	B 4,4'-DDE	6.204	5.218	320.2E6	156.6E6	111.815	115.040
13)	MA Dieldrin	6.359	5.349	356.3E6	180.5E6	114.312	113.792
14)	MA Endrin	6.589	5.625	284.6E6	153.9E6	111.925	110.861
15)	B Endosulfa...	6.809	5.919	294.2E6	151.8E6	104.100	113.418
16)	A 4,4'-DDD	6.723	5.773	258.6E6	125.8E6	118.978	126.502
17)	MA 4,4'-DDT	7.038	6.024	267.1E6	127.5E6	121.057	123.179
18)	B Endrin al...	6.939	6.099	212.8E6	109.6E6	98.879	100.889
19)	B Endosulfa...	7.174	6.322	244.6E6	136.6E6	98.282	109.066
20)	A Methoxychlor	7.514	6.599	689.2E6	322.6E6	535.736	571.925
21)	B Endrin ke...	7.660	6.829	316.0E6	168.4E6	112.273	114.423

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083123\
Data File : PD077473.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2023 12:41
Operator : AR\AJ
Sample : 04123-09MSD
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 21:28:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 01:53:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

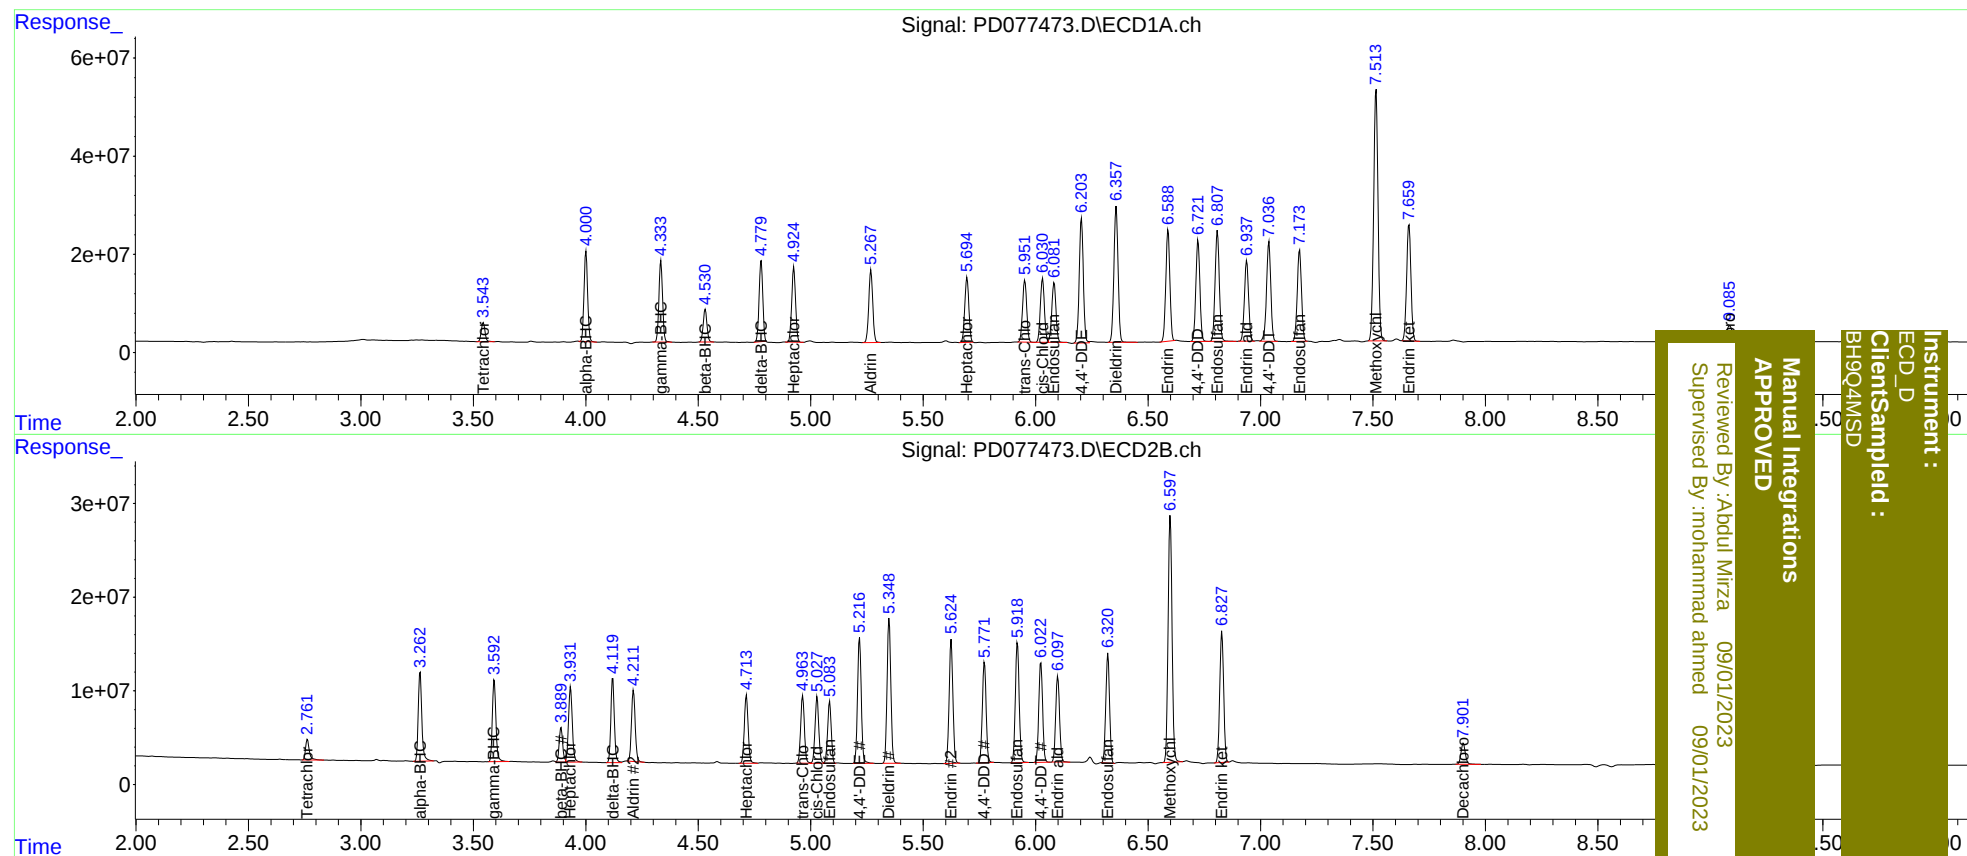

Instrument :
ECD_D
ClientSampled :
BH9Q4MSD

Manual Integrations
APPROVED

Reviewed By :Abdul Miza 09/01/2023
Supervised By :mohammad ahmed 09/01/2023