

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083124\
 Data File : PD084832.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2024 16:38
 Operator : AR\AJ
 Sample : P3721-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCYD8

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/03/2024
 Supervised By : Ankita Jodhani 09/03/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 03:19:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.905	11614399	47683431	11.483	13.474m
2)	SA Decachlor...	9.035	8.107	13632185	52192495	10.438	15.010 #
Target Compounds							
13)	MA Dieldrin	6.325	5.548	1828900	5675966	1.240m	1.321m
15)	B Endosulfa...	6.760	6.106	1633205	3437401	1.237m	0.927m#
20)	A Methoxychlor	7.464	6.784	544263	7051782	1.045m	4.263m#
21)	B Endrin ke...	7.587	7.030	2095251	9985925	1.714m	2.268m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083124\
Data File : PD084832.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2024 16:38
Operator : AR\AJ
Sample : P3721-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 03:19:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

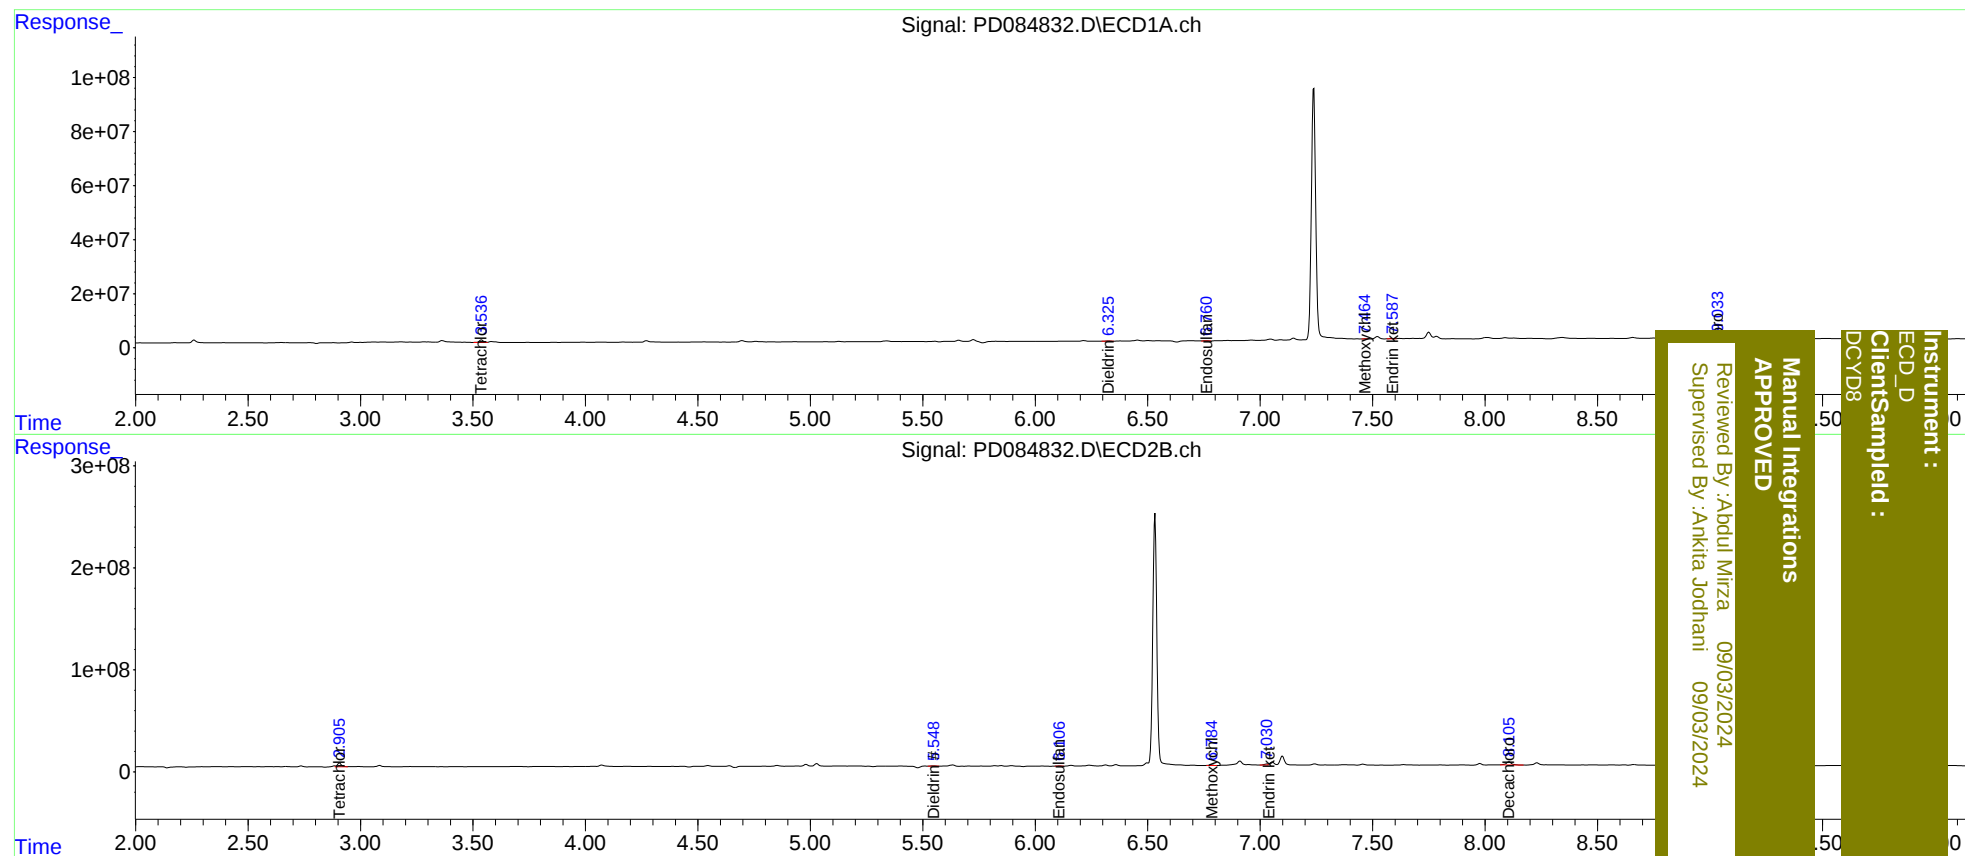

Reviewed By: Abdul Mirza 09/03/2024
Supervised By: Ankita Jodhani 09/03/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
DCYD8