

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083124\
 Data File : PD084836.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2024 17:31
 Operator : AR\AJ
 Sample : P3721-08MS
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCXZ0MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/30/2024
 Supervised By : Ankita Jodhani 09/03/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 03:20:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	2.905	13978309	55303497	13.821m	15.628m
27)	SA Decachlor...	9.033	8.106	16595260	57446674	12.707	16.521 #
Target Compounds							
2)	A alpha-BHC	3.984	3.418	92395613	264.7E6	54.345	52.206
3)	MA gamma-BHC...	4.312	3.753	88156947	253.9E6	54.490	52.403
4)	MA Heptachlor	4.910	4.107	85226295	227.1E6	55.392	53.337
5)	MB Aldrin	5.250	4.393	81075882	220.8E6	50.693	49.713
6)	B beta-BHC	4.495	4.044	34831384	106.0E6	47.953	48.877m
7)	B delta-BHC	4.742	4.283	86758220	253.6E6	52.901	51.083
8)	B Heptachlo...	5.669	4.897	71068820	200.9E6	47.650	47.437
9)	A Endosulfan I	6.050	5.271	65473599	189.5E6	47.589m	49.440m
10)	B trans-Chl...	5.923	5.149	67951400	207.6E6	48.180	50.462m
11)	B cis-Chlor...	6.002	5.216	69421744	202.4E6	46.952m	48.231
12)	B 4,4'-DDE	6.173	5.401	127.1E6	395.9E6	101.867	100.936
13)	MA Dieldrin	6.324	5.540	143.2E6	420.3E6	97.050	97.828
14)	MA Endrin	6.551	5.817	123.4E6	396.3E6	109.358	107.047
15)	B Endosulfa...	6.761	6.108	120.4E6	343.4E6	91.246	92.605
16)	A 4,4'-DDD	6.681	5.958	103.1E6	295.4E6	104.420	87.047
17)	MA 4,4'-DDT	6.996	6.212	100.5E6	316.3E6	112.263	98.881
18)	B Endrin al...	6.888	6.286	88308101	256.4E6	97.783m	89.796m
19)	B Endosulfa...	7.123	6.512	115.9E6	321.9E6	100.564	90.122
20)	A Methoxychlor	7.466	6.784	287.1E6	753.9E6	551.079	455.704
21)	B Endrin ke...	7.603	7.023	119.5E6	385.9E6	97.739	87.633

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083124\
Data File : PD084836.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2024 17:31
Operator : AR\AJ
Sample : P3721-08MS
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 03:20:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

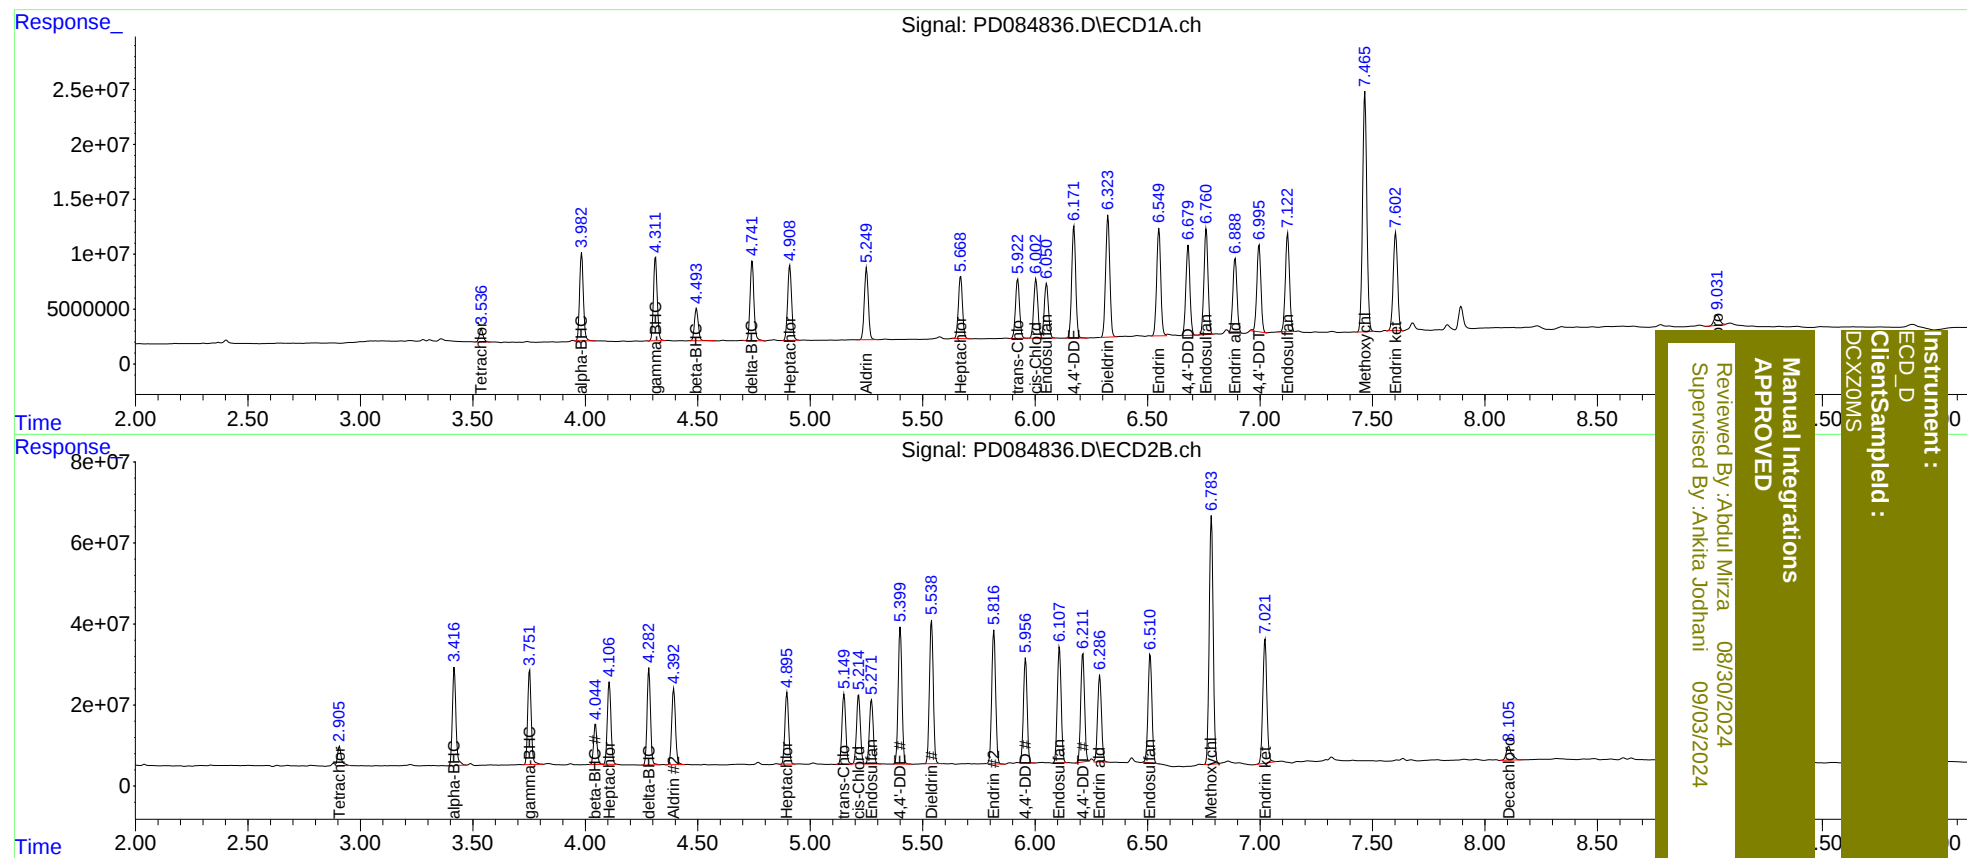

Instrument :
ECD_D
ClientSampled :
DCXZ0MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 08/30/2024
Supervised By: Ankita Jodhani 09/03/2024