

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083124\
 Data File : PD084837.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Aug 2024 17:45
 Operator : AR\AJ
 Sample : P3721-09MSD
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCXZ0MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/03/2024
 Supervised By : Ankita Jodhani 09/03/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 30 03:20:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	2.905	14192594	54837373	14.033m	15.496m
2)	SA Decachlor...	9.032	8.106	19516485	59850180	14.943	17.212
Target Compounds							
2)	A alpha-BHC	3.983	3.417	91567081	261.6E6	53.858	51.590
3)	MA gamma-BHC...	4.312	3.752	88426712	252.5E6	54.657	52.101
4)	MA Heptachlor	4.910	4.107	80639260	226.3E6	52.411	53.161
5)	MB Aldrin	5.250	4.392	78712182	222.7E6	49.215	50.147m
6)	B beta-BHC	4.495	4.044	33602655	104.2E6	46.261	48.047m
7)	B delta-BHC	4.742	4.283	83458648	251.8E6	50.889	50.718
8)	B Heptachlo...	5.669	4.897	76829145	200.5E6	51.512	47.331
9)	A Endosulfan I	6.050	5.271	67253188	167.6E6	48.883m	43.730m
10)	B trans-Chl...	5.923	5.151	69872859	205.0E6	49.542	49.830
11)	B cis-Chlor...	6.003	5.216	71515083	204.4E6	48.368m	48.715
12)	B 4,4'-DDE	6.173	5.401	133.1E6	395.6E6	106.684	100.841
13)	MA Dieldrin	6.324	5.540	149.5E6	418.4E6	101.363	97.391
14)	MA Endrin	6.549	5.817	128.2E6	399.0E6	113.613m	107.770
15)	B Endosulfa...	6.761	6.109	121.3E6	343.1E6	91.882	92.549
16)	A 4,4'-DDD	6.681	5.958	107.7E6	292.7E6	109.046	86.254
17)	MA 4,4'-DDT	6.996	6.213	100.0E6	313.3E6	111.742	97.938
18)	B Endrin al...	6.889	6.288	80116222	240.3E6	88.712	84.158
19)	B Endosulfa...	7.123	6.512	116.1E6	334.9E6	100.759	93.781
20)	A Methoxychlor	7.466	6.784	292.1E6	800.7E6	560.734	483.998
21)	B Endrin ke...	7.603	7.022	127.0E6	395.7E6	103.848	89.858

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD083124\
Data File : PD084837.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Aug 2024 17:45
Operator : AR\AJ
Sample : P3721-09MSD
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 30 03:20:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

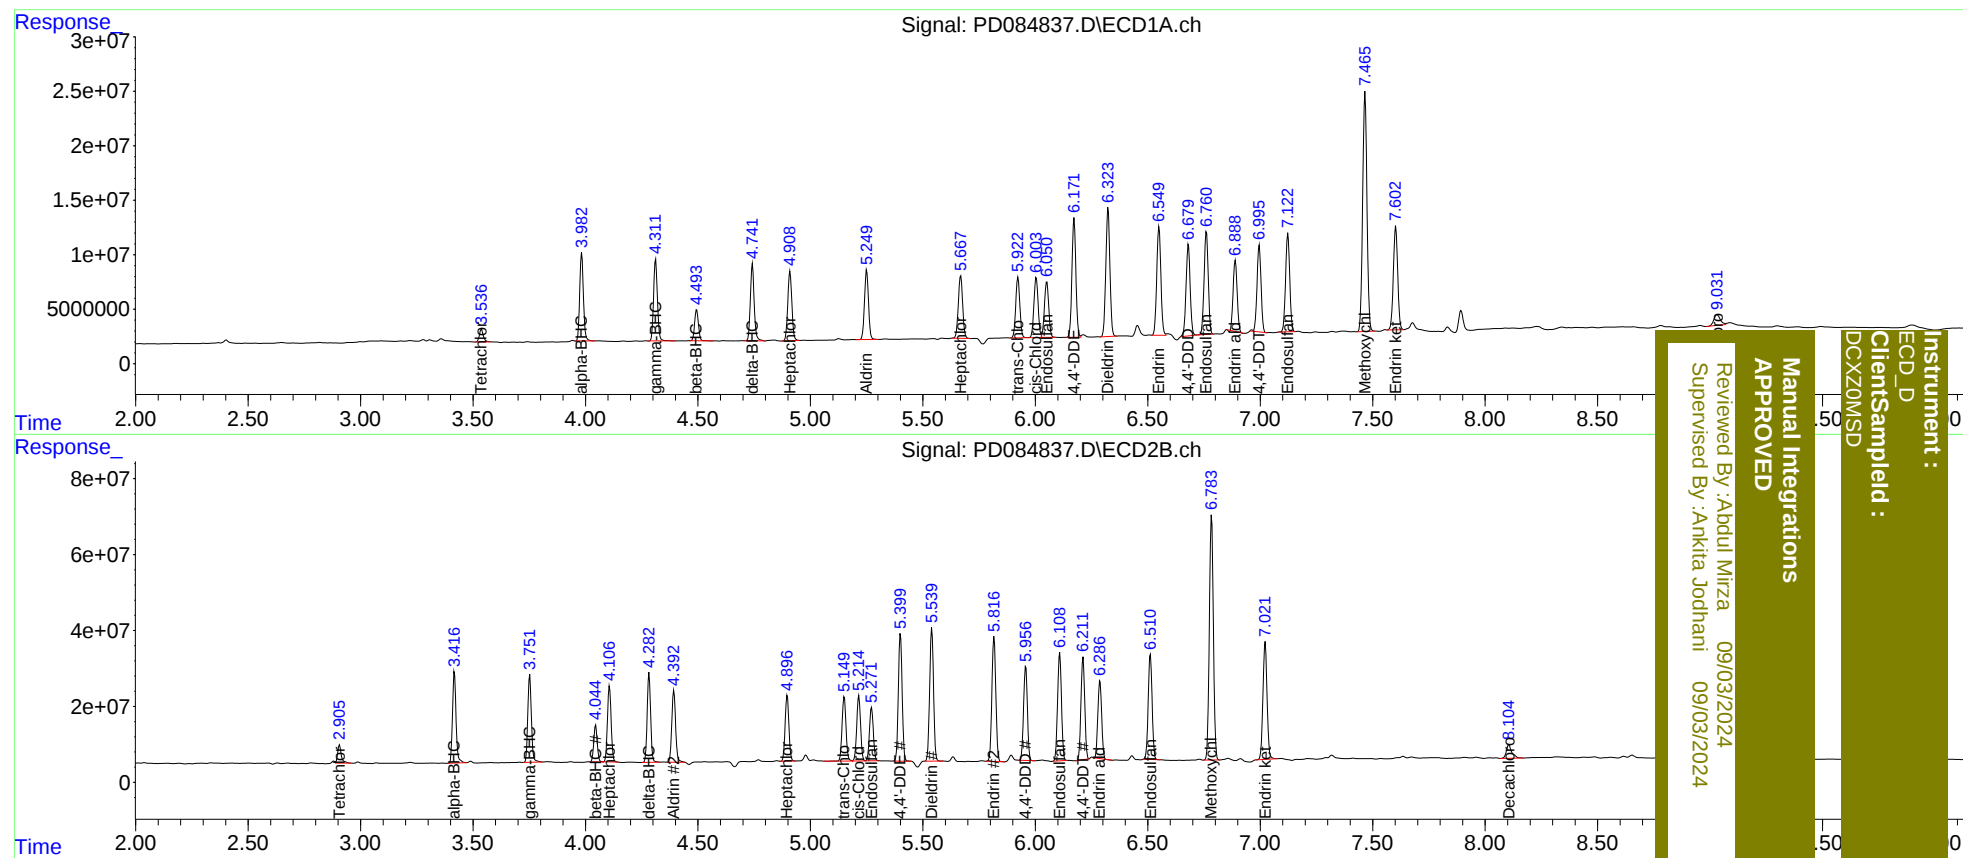

Instrument :
ECD_D
Client Sampled :
DCXZ0MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 09/03/2024
Supervised By: Ankita Jodhani 09/03/2024