

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090121\
 Data File : PD065489.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2021 10:15
 Operator : AR\AJ
 Sample : M3263-01
 Misc : PEST MDL 1 PPB
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-QT4-2021-07

Manual Integrations
 APPROVED

mohammad
 9/8/2021 2:38:14 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 08:10:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082921CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 28 03:49:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.014	21198761	144.7E6	18.752	17.857
2)	SA Decachlor...	8.242	9.087	50530884	188.9E6	34.978	36.530
Target Compounds							
2)	A alpha-BHC	3.935	4.409	2160402	13359364	1.403	1.223
3)	MA gamma-BHC...	4.218	4.695	2160646	12720273	1.321m	1.209
4)	MA Heptachlor	4.516	5.200	1932657	11175757	1.318m	1.111
5)	MB Aldrin	4.765	5.505	1876550	12292959	1.329	1.285
6)	B beta-BHC	4.468	4.871	1670471	6189411	2.265m	1.289m#
7)	B delta-BHC	4.672	5.089	1907676	15832176	1.270	1.536
8)	B Heptachlo...	5.207	5.895	1926935	3708814	1.429	0.455 #
9)	A Endosulfan I	5.545	6.253	1692770	9684449	1.328	1.306
10)	B trans-Chl...	5.431	6.127	1750699	10114546	1.278m	1.247m
11)	B cis-Chlor...	5.491	6.200	1850173	10287472	1.360	1.298
12)	B 4,4'-DDE	5.654	6.358	1560049	9447102	1.247	1.277
13)	MA Dieldrin	5.789	6.508	1758048	11737439	1.314	1.534m
14)	MA Endrin	6.047	6.729	1841201	8722644	1.512	1.377
15)	B Endosulfa...	6.318	6.942	2049103	8343156	1.627m	1.287
16)	A 4,4'-DDD	6.168	6.851	1389025	8266248	1.266m	1.373m
17)	MA 4,4'-DDT	6.408	7.150	1543082	7556348	1.286m	1.239
18)	B Endrin al...	6.488	7.067	1605179	8312010	1.601	1.624
19)	B Endosulfa...	6.699	7.290	2338932	7865855	1.828	1.266 #
20)	A Methoxychlor	6.956	7.609	825794	4045686	1.263	1.386
21)	B Endrin ke...	7.194	7.762	2122996	10442879	1.366	1.470m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090121\
Data File : PD065489.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2021 10:15
Operator : AR\AJ
Sample : M3263-01
Misc : PEST MDL 1 PPB
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 08:10:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082921CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 28 03:49:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

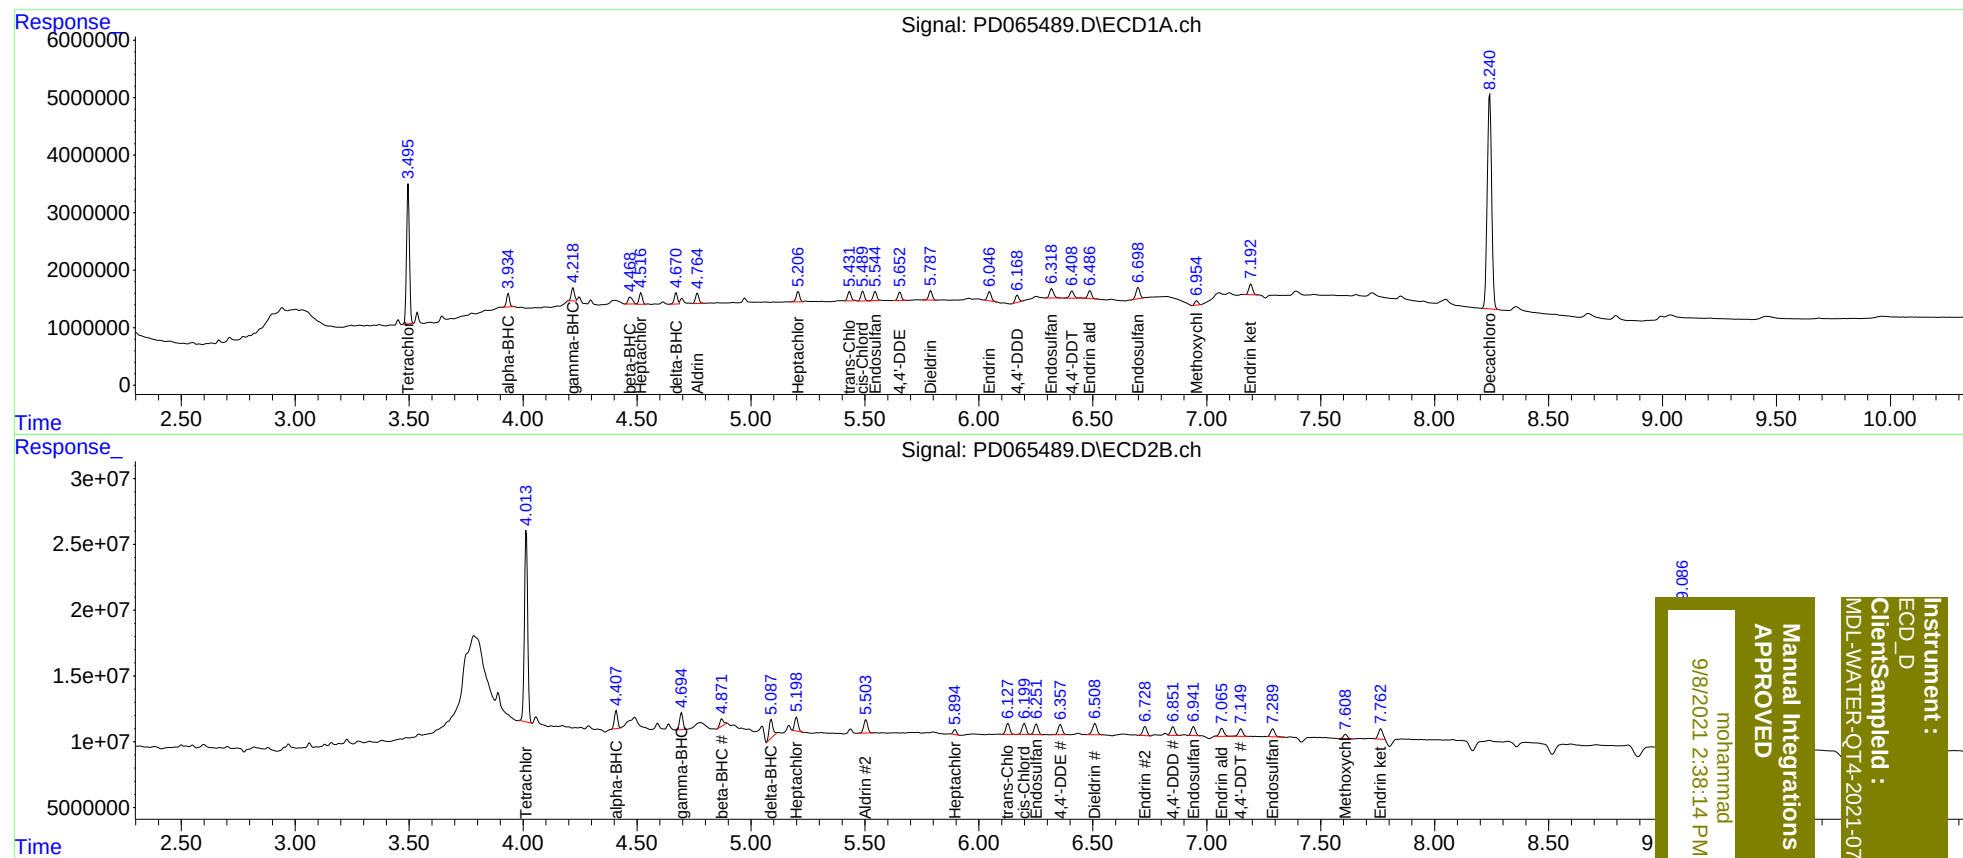

Manual Integrations
APPROVED

mohammad
9/8/2021 2:38:14 PM

Instrument :
ECD_D
Client Sample :
MDL-WATER-QT4-2021-07